



EUDAMED user guide

UDI Devices

Playground v 3.27.2
2026

ground

Table of Contents

1. Introduction	1
2. Getting started	4
3. Register Regulation Devices	6
3.1. Register a Basic UDI-DI together with a UDI-DI of a Regulation Device	7
3.1.1. Step 1: Enter the device and its Basic UDI-DI information	7
3.1.2. Step 2: Enter certificate information (if applicable)	11
3.1.3. Step 3: Enter UDI-DI identification information ...	12
3.1.4. Step 4: Enter UDI-DI characteristics	21
3.1.5. Step 5: Enter additional device information	24
3.1.6. Step 6: Enter container package details	29
3.2. Register a regulation device and its UDI-DI for an existing Basic UDI-DI	32
4. Register System or Procedure Packs (SPP)	36
4.1. Register Basic UDI-DI together with a UDI-DI for a System or Procedure Pack	36
4.1.1. Step 1: Enter SPP and Basic UDI-DI main information	36
4.1.2. Step 2: Basic UDI-DI information	37
4.1.3. Step 3: UDI-DI identification information	39
4.1.4. Step 4: UDI-DI characteristics	45
4.1.5. Step 5: Container package details	47
4.2. Register a new System or Procedure Pack UDI-DI for an existing Basic UDI-DI	49
4.2.1. Step 1: UDI-DI identification information	50
4.2.2. Step 2: UDI-DI characteristics	52
4.2.3. Step 3: Container package details	52
5. Manage your Device information	53
5.1. Manage your device details and Basic UDI-DI/EUDAMED DI	53
5.1.1. Delete draft Basic UDI-DI/EUDAMED DI	54

5.1.2. Update (create new version of the record) for Basic UDI-DI/EUDAMED DI	55
5.1.3. View historical versions of device data and its Basic UDI-DI/EUDAMED DI	57
5.2. Manage your device UDI-DI/EUDAMED ID details	58
5.2.1. Delete draft UDI-DI/EUDAMED ID	60
5.2.2. View details of a registered device and its UDI-DI/EUDAMED ID details	61
5.2.3. Update (create a new version) for a device and its UDI-DI/EUDAMED ID	68
5.2.4. Update Product original manufacturer	73
5.2.5. Update Market Information	75
5.2.6. Update Container Packages	76
5.2.7. Discard registered devices and their UDI-DIs/ EUDAMED-IDs (and their Basic UDI-DI/EUDAMED-DI	81
5.2.8. Link registered Regulation Device to registered Legacy Device	82
5.2.9. Delete link between Regulation Device and Legacy Device	85
5.2.10. View historical versions of a device and its UDI-DI/EUDAMED-ID and associated entities	86
6. Manage your own System or Procedure Pack (SPP) information	88
6.1. Manage your SPP Basic UDI-DI details	88
6.1.1. Delete a SPP draft Basic UDI-DI	89
6.1.2. Update SPP Basic UDI-DI	90
6.1.3. View SPP Basic UDI-DI historical versions	92
6.2. Manage your SPP UDI-DI details	93
6.2.1. Delete SPP draft UDI-DI	94
6.2.2. Update SPP UDI-DI	95
6.2.3. Update SPP Container Packages	97
6.2.4. Discard SPP registered UDI-DIs	99
6.2.5. View SPP historical versions for UDI-DI and associated entities	101
7. Search & View Devices and Systems or Procedure Packs	102

7.1. Search & View sub-statuses of Devices or SPPs	104
7.2. Search & View historical versions of Devices or SPPs	106
7.3. Download Devices or SPPs data in a structured format (XML)	108
7.4. View historical versions of Basic UDI-DI/EUDAMED DI, UDI-DI/EUDAMED ID and associated entities	109
8. Annex – device certificate information	113

Playground

1 Introduction

Regulation (EU) 2017/745 on medical devices and Regulation (EU) 2017/746 on *in vitro* diagnostic medical devices introduce an EU identification system for medical devices based on a Unique Device Identifier (UDI).

The UDI-DI/Device module of EUDAMED is used for the manufacturers to provide their UDIs/Devices information and ensure its availability to everyone. Moreover, it is used to manage the registration of devices and systems and procedure packs (SPPs) across the EU/EEA.

It falls within the responsibilities of manufacturers (MFs) of devices and system and procedure pack producers (SPPPs) to ensure product registration in the UDI/Device Module. Authorised Representatives and Importers cannot register devices or SPPs. The devices to be registered are defined by Article 2 in MDR and IVDR. UDI-DI/Device module of EUDAMED is used for the manufacturers to provide information on the devices and the corresponding UDIs and to make it available to everyone.



TIP

For a wider understanding on how to use the platform visit the [EUDAMED Information Centre](#). For information specific to UDIUDI, visit the [UDI Helpdesk](#).



NOTE

This user guide outlines the registration of medical devices, IVD medical devices, SPPs, the device data, including the corresponding Basic UDI-DI and UDI-DI.



Economic Operators (EOs) must register their organisation in the Actor (ACT) module before they are given access to EUDAMED and become able to register their devices and SPPs in the UDI/Devices module. See the [EOs User Guide](#). Devices and SPPs must be registered in the UDI/Devices module before they are placed on the union market (see [Q&A on EUDAMED gradual roll out](#)). Device registration does not involve any assessment, review or approval by a Competent Authority (CA). Some of the information in EUDAMED is publicly available for searching and viewing.

**WARNING**

- The requirements for device registration differ, depending on when the device is placed on the market and depending on which legislation it is compliant with ("regulation devices", "legacy devices", "old devices" – see [Q&A on EUDAMED gradual roll out](#)).
- In EUDAMED, device/SPP registration in the UDI/Devices module means registering a device/SPP at the level of the device identifier. Production identifiers are not required.
- EUDAMED does not contain all constraints defined in the MDR/IVDR, guidance and good practices, and therefore, it is not because something is possible in EUDAMED that it is necessarily allowed.

**VIDEO: What is a UDI?**

Please note that this video contains sound.

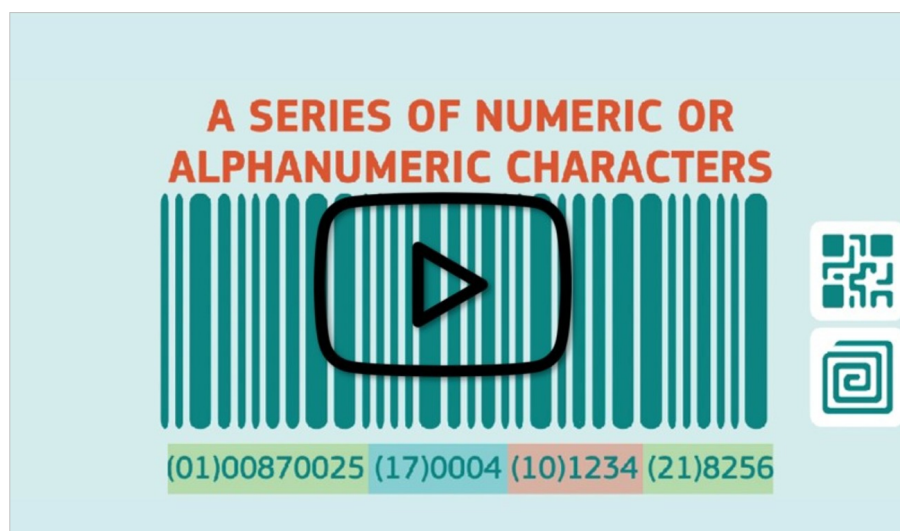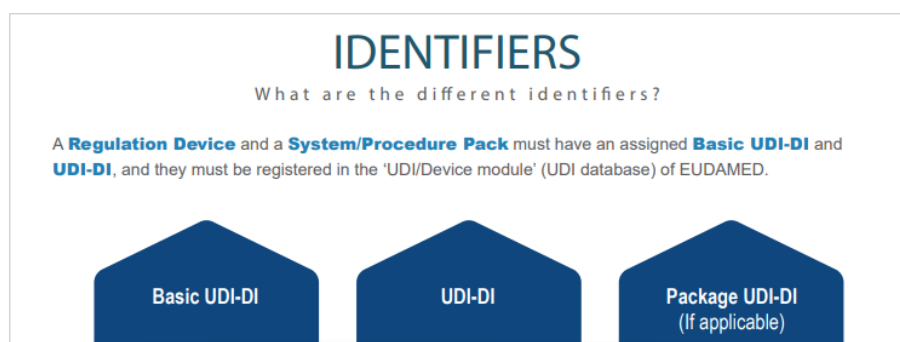**INFOGRAPHIC: Basic UDI-DI/UDI-ID concept**

**CAUTION**

In case a serious incident occurs and Vigilance reporting is required in the VGL module of EUDAMED, this cannot be done before the device is registered in the UDI/ Devices module. If the incident involves a device that is not mandatory to be registered in EUDAMED (old device, custom-made device), there is an alternate registration procedure available for entering limited device data. These are referred to as “old/ custom-made” (OCMs).

Playground

2 Getting started

What I need to access EUDAMED

1. [EU Login \(ECAS\) account](#):

To use EUDAMED, you must have an EU Login account associated with your professional email address and the manufacturer for which you want to act on behalf must be registered as an actor in EUDAMED.

2. User profile registration in EUDAMED:

For information on how to gain access to EUDAMED, please consult the [Economic Operators user guide](#).

Every user in EUDAMED is granted by default the profile *Viewer* for the UDI/Device module, and can search and view registered devices. However, to enter data on the devices and their UDIs in EUDAMED, your profile for the UDI/Device module ¹ must be either:

- A *Proposer* – this profile allows you to create and delete draft records related to your manufacturer, but not to submit a device, or
- A *Confirmer* – this profile includes the *Proposer* rights and additionally, allows you to submit and discard records. Moreover, it allows you to directly register a device.



NOTE

See the [Economic Operators user guide](#), Section *Upgrading your user profile* for further information on how to upgrade your profile from *Viewer* to *Proposer* or *Confirmer*.



IMPORTANT

A Local Actor Administrator (LAA)/Local User Administrator (LUA) of your manufacturer must approve your user access request (If you don't have a second user with LAA/LUA profile, please refer to the [Economic Operators user guide](#), Section *Requesting access as a second LAA user to an existing registered actor*).

Before you start entering details of a UDI/device in EUDAMED, please ensure you have all the required information at hand, including the Basic UDI-DI and UDI-DI codes. Fields marked with a red asterisk are mandatory.

Once you enter information into EUDAMED, it may not be possible to change it, if entered incorrectly. Certain fields are not editable after submission of the record.

¹See the [Economic Operators user guide](#), Section *User rights and profiles*, for more information on user rights and profiles.



NOTE

EUDAMED user interface is available in all EU languages and the information can be entered in any official language within the EU.

Playground

3 Register Regulation Devices

VIDEO: Registering Regulation Devices

Please note that this video does not contain sound.



NOTE

- Devices or SPPs to be placed on the market according to MDR/IVDR (“regulation devices”) must first be registered in the UDI/Devices module together with their UDI and other device data;
- Each Regulation Device must have a unique Basic UDI-DI and a unique UDI-DI assigned to it. Both are always required – you cannot register a Basic UDI-DI without a UDI-DI

You will be asked to log into EUDAMED via your EU Login account. This will take you to the actor (manufacturer, system/procedure pack producer) to which you are connected through your user account. If you have user accounts for more than one actor, your options will be available on the screen. Choose the appropriate one by clicking on the actor name.




INFOGRAPHIC: [UDI registration for regulation devices](#)



3.1 Register a Basic UDI-DI together with a UDI-DI of a Regulation Device


 **INFOGRAPHIC:** [Basic UDI-DI/UDI-ID concept](#)

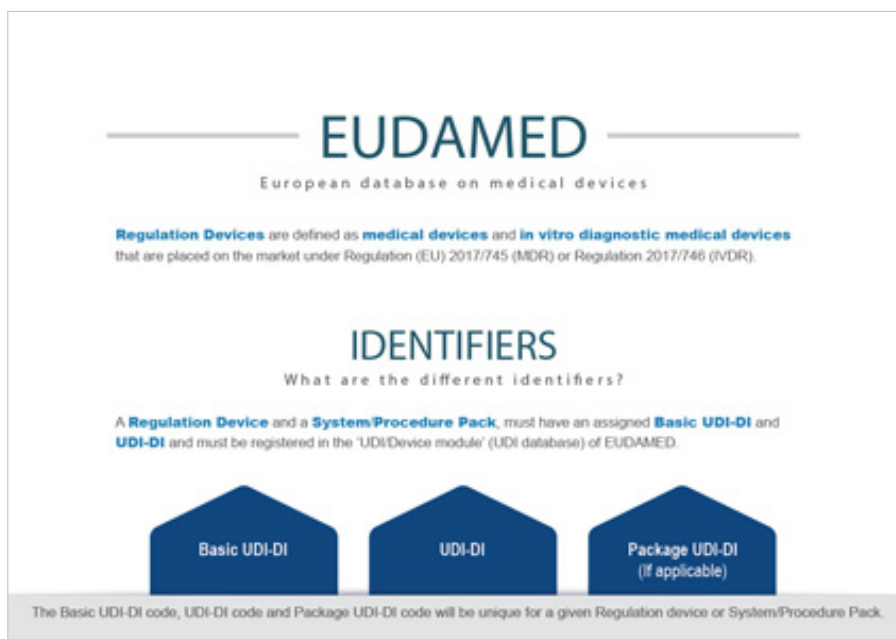

3.1.1 Step 1: Enter the device and its Basic UDI-DI information

 **VIDEO:** UDI and medical software devices

Please note that this video contains sound.

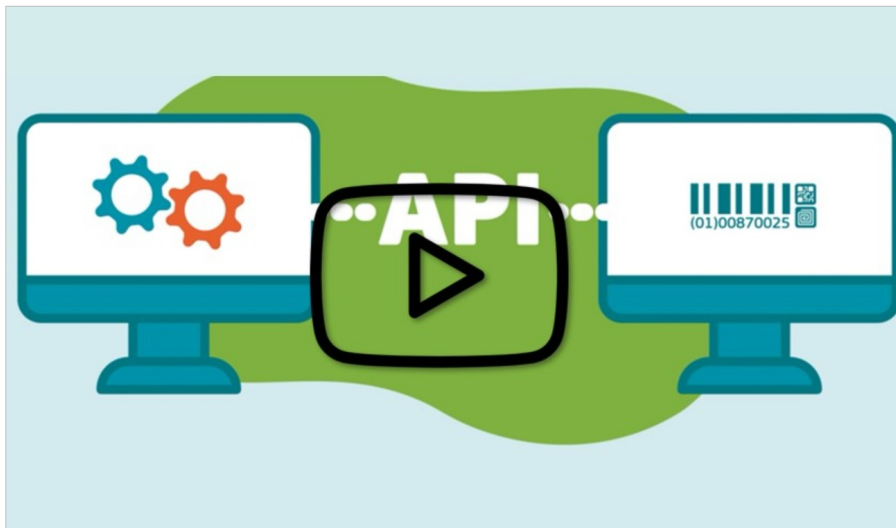

1. Click on *Register a new Basic UDI-DI*:

Tasks
By module, consult, verify and/or manage your own and related data (managed by your actor), depending on your profile.

My Actor data	UDI-DIs/Device	User management
Manage your actor data Manage your email notifications	Register a new Basic UDI-DI Register a legacy device Manage your Basic UDI-DIs / EUDAMED DIs Manage your Devices details	Assess user access requests Manage your users

2. Enter the Basic UDI-DI information and select the applicable regulation for your device:



NOTE

In this guide, the selection is MDR (Regulation (EU) 2017/745). Based on the regulation you choose, the characteristics of the Device to be entered will vary.

UDI-DI registration

Manufacturer identification

Organisation name:	Test MF
Actor ID/SRN:	LI-MF-000000104
Address:	Oak St, 101 8088 Vaduz
Telephone number:	+343 8987 65 13
Email:	eudamed@manufacturer.com

*** Applicable regulation**

☐ MDR (REGULATION (EU) 2017/745 on medical devices)
☐ IVDR (REGULATION (EU) 2017/746 on in vitro diagnostic medical devices)

Depending on the regulation selected an additional question appears at the bottom of the page:

Regulation	Additional question
MDR	<i>Is it a System or Procedure Pack which is a Device in itself?</i> + additional sub-questions about the device type, depending on whether your answer is Yes or No to this first question
IVDR	<i>Is it a kit?</i> + additional sub-question about the device type, if you answer No to this first question

Is it a System or Procedure Pack which is a Device in itself?

Yes ☒ No ☐  Is it a System or Procedure Pack which is a Device in itself is required unless you select the option - No

☐ Procedure Pack which is a Device in itself

☐ System which is a Device in itself

If you select **No**, please choose the right information under the appearing section *Special Device type* (for IVDR, if you select **No** for *Is it a Kit?*, the only option for Special device type if applicable is *Software*² (See video above):

Special device type

Yes ☒ No ☐  Special device type is required unless you select the option - No

*** Special device type:**

☐ Software

☐ Standard soft contact lenses

☐ Standard Rigid Gas Permeable (RGP) contact lenses

☐ Made to order soft contact lenses

☐ Made to order Rigid Gas Permeable (RGP) contact lenses

☐ Spectacle frames

☐ Spectacle lenses

☐ Ready-made reading spectacles



NOTE

For certain MDR device types, the registration of a UDI-DI is not appropriate. If one of the following Special Device types is selected, the Master UDI-DI applies instead:

- Standard soft contact lenses
- Standard Rigid Gas Permeable (RGP) contact lenses
- Made to order soft contact lenses
- Made to order Rigid Gas Permeable (RGP) contact lenses.

²For more information, visit the EUDAMED Information Centre, or the [UDI Assignment to Medical Device Software](#) webpage.

**NOTE**

Currently, it is not possible to select certain devices. If one of the following Special Device types is selected, the system will block you from saving the registration:

- Spectacle frames;
- Spectacle lenses;
- Ready-made reading spectacles

It is not possible to register these devices through Machine-to-machine or Bulk uploads either.

3. Fill in the Basic UDI-DI identification details and click **Save & Next**:

Basic UDI-DI main information

* Issuing Entity:

* Basic UDI-DI code:

Save & Next >

**IMPORTANT**

EUDAMED will validate the Basic UDI-DI code based on the specific format for each Issuing Entity and will prevent you from going further if the code is not valid. However, EUDAMED cannot verify that the code is correct beyond the format.

If the Basic UDI-DI code already exists in EUDAMED, the system will prevent you from saving, as a Basic UDI-DI must be unique. Once you save your changes, you will not be able to amend the information at a later stage.

4. Non-EU manufacturers will have to select the Authorised Representative for the Basic UDI-DI amongst those with which they have an active mandate registered in EUDAMED.

If there is only one Authorised Representative with an active mandate with the non-EU Manufacturer, it will be automatically retrieved:

Authorised representative identification

Organisation name: Belgian AR A

Eudamed actor ID: BE-AR-000000046

Address: Rue E, 1 1060 Brussels

Telephone number: -

Email: contact@belgian-ar-a.be

5. Choose a corresponding Risk Class and select **Yes** or **No** for each option that follows:

Basic UDI-DI information

* Risk class:

* Measuring function

☐ Yes ☐ No

* Active device

☐ Yes ☐ No

* Device intended to administer and/or remove medicinal product

☐ Yes ☐ No

6. Select **Yes** or **No** if Device model is applicable. If you selected *No*, the Device Name will be mandatory, otherwise, it is mandatory to enter the Device model and the Device name (at the Basic UDI-DI level) if there is one (note that the device trade name is part of the UDI-DI data):

Device model applicable

Yes ☒ No ☐ Device model is required by default unless you select the option - No

* Device model:

Device Model_Test

Device Name:

7. Click **Save** to save your registration as a draft and continue later, or **Save & Next** to save it as a draft and continue directly with the following steps:

Save **Save & Next >**

3.1.2 Step 2: Enter certificate information (if applicable)

This section only becomes accessible depending on the Risk Class information provided and additional properties in the Basic UDI-DI and applies to certificates issued by the Notified Bodies (NBs).



NOTE

Certificate Information for registration of a device and its Basic UDI-DI registration is applicable only when its confirmation by the Notified Body from the certificate registration is required (as specified in Art 29(3) MDR/Art 26(2) IVDR).


In [Annex – Device Certificate Information \[113\]](#) you can find the different cases in which Certificate information is required and the type of certificate.

For certificate information, at least the following should be provided:

- whether *EU type examination certificate* is applicable.
- the Notified Body (NB) responsible for the product certificate.
- if known, the certificate identification.

Additionally, more information on the certificate type could be required depending on the risk class and properties specified for the Basic UDI-DI. For the NB, enter some or all of the NB name or number, click **Find** and choose the correct NB from the new window. EUDAMED does not verify whether the NB is the right one for your device.

If known, enter the certificate number and revision number and click **Save** or **Save & Next**.

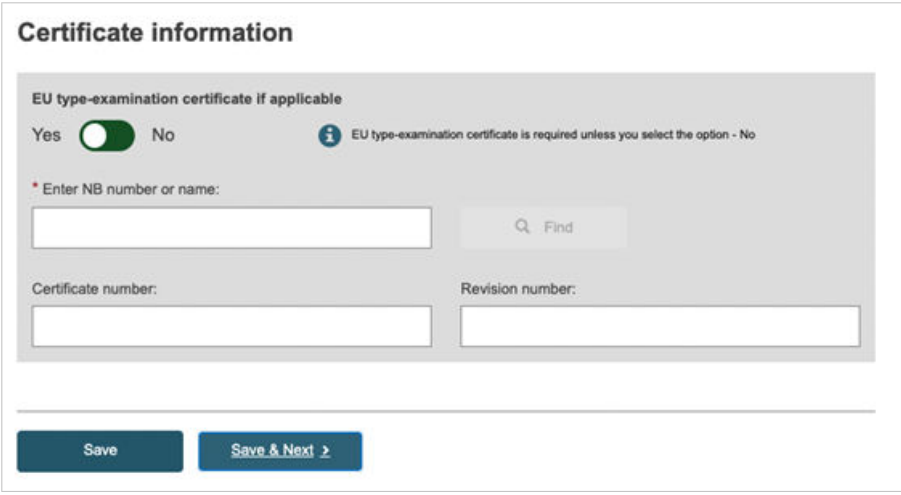

The screenshot shows a web form titled "Certificate information". It contains a section for "EU type-examination certificate if applicable" with a "Yes" toggle (currently turned on) and a "No" option. A tooltip indicates that the certificate is required unless "No" is selected. Below this is a text input field for "Enter NB number or name:" with a "Find" button. At the bottom, there are two input fields for "Certificate number:" and "Revision number:". At the very bottom of the form are two buttons: "Save" and "Save & Next >".



NOTE

Notifications to MFs and ARs

When a new Product Certificate has been registered in EUDAMED both the MF and, if applicable, the AR are notified.

3.1.3 Step 3: Enter UDI-DI identification information



VIDEO: UDI carrier and display formats

Please note that this video does not contain sound.



1. Select the *Issuing Entity* from the drop-down list and enter the *UDI-DI code*.



IMPORTANT

The UDI-DI code you enter must be unique. If it already exists in EUDAMED, you will not be able to Save.

Exception: the same UDI-DI can be used for a Legacy Device and its Regulation Device equivalent from the same manufacturer.

If the same UDI-DI code was already provided for a Legacy Device (i.e. applicable legislation MDD, AIMDD or IVDD), you will be prompted that a link will be created between the two devices (the Regulation and the Legacy Device) on the condition there is no conflict between some of the Basic UDI-DI properties and the related legacy device EUDAMED DI properties. In case of conflict, the system will prevent you from using the same UDI-DI.



NOTE

In the case your chosen Issuing Entity is **GS1**, the UDI-DI code you enter must be a 14-digit code including the check digit that will be used by EUDAMED to validate the UDI-DI code. If your GS1 UDI-DI (GTIN code) is shorter than 14 digits (check digit included), when populating EUDAMED field please add leading zero(s) until you reach 14 digits.

For example:

000000nnnnnnnnn (GTIN-8)

00nnnnnnnnnnnnnn (GTIN-12)

0nnnnnnnnnnnnnnn (GTIN-13)

**NOTE**

When registering a Master UDI-DI code, a specific format validation algorithm is applied when the issuing entity is GS1:

- For **Standard soft contact lenses** and **Standard Rigid Gas Permeable (RGP) contact lenses** the system applies the GMN format validation algorithm.
- For **Made-to-order soft contact lenses** and **Made-to-order Rigid Gas Permeable (RGP) contact lenses** the system applies the GTIN UDI-DI format validation algorithm.

2. If applicable, enter the Secondary UDI-DI from a different Issuing Entity to the UDI-DI:

UDI-DI identification

UDI-DI identification

* Issuing Entity: * UDI-DI code:

UDI-DI from another entity (secondary) applicable

Yes ☒ No ☐ UDI-DI from another entity is required unless you select the option - No

* Issuing Entity: * Secondary UDI-DI value:

**NOTE**

Secondary UDI-DI may exist due to the fact that the manufacturer changed issuing entity. The UDI-DI assigned to the device being registered from the previous issuing entity can be referenced in EUDAMED together with the new one.

3. Enter the EMDN code, click **Find** and select the correct one from the list:

* Enter a nomenclature code (EMDN code):

[Advanced search of device nomenclature](#)

Selected nomenclature codes

[Code A0101010101](#) HYPODERMIC SYRINGE NEEDLES, WITH SAFETY SYSTEMS

**NOTE**

MDR and IVDR require that an internationally recognised medical devices nomenclature is used when registering devices in EUDAMED. The nomenclature to be used according to MDR/IVDR is EMDN.

**NOTE****Search for Nomenclature codes (EMDN)**

Click on **Advanced search of device nomenclature** to search by partial code name and view the list of codes alphabetically:

Find the code ✕ Close

EMDN Code: EMDN Description:

A DEVICES FOR ADMINISTRATION, WITHDRAWAL AND COLLECTION

A01 NEEDLES

A0101 NEEDLES FOR INFUSION AND SAMPLING

A010101 HYPODERMIC NEEDLES

A01010101 HYPODERMIC SYRINGE NEEDLES

- ☐ A0101010101 HYPODERMIC SYRINGE NEEDLES, WITH SAFETY SYSTEMS
- ☐ A0101010102 HYPODERMIC SYRINGE NEEDLES, W/O SAFETY SYSTEMS

A01010102 HYPODERMIC PEN NEEDLES

- ☐ A0101010201 HYPODERMIC PEN NEEDLES, WITH SAFETY SYSTEMS
- ☐ A0101010202 HYPODERMIC PEN NEEDLES, W/O SAFETY SYSTEMS

- ☐ A01010199 HYPODERMIC NEEDLES - OTHER
EMDN Code updates

EMDN codes may get updated and therefore have a version history, which is indicated by an *information* icon.

Click on the *information* icon to view details about a code's versions and status:

Playground

UDI-DI from another entity (secondary) applicable

Find the code

EMDN Code: EMDN Description:

ⓘ Nomenclature already selected

B010101 AUTOLOGOUS BLOOD COLLECTION BAGS

B01010101 AUTOTRANSFUSION BAGS, WITH FILTERS AND KITS

☐ B0101010101 AUTOTRANSFUSION DOUBLE BAGS, WITH FILTERS AND KITS ⓘ

☐ B0101010199 AUTOTRANSFUSION BAGS, WITH FILTERS AND KITS

B01010102 AUTOTRANSFUSION BAGS, WITH FILTERS AND KITS

☐ B0101010201 AUTOTRANSFUSION BAGS, WITH FILTERS AND KITS

☐ B0101010202 AUTOTRANSFUSION DOUBLE BAGS, W/O FILTERS AND KITS

☐ B0101010203 AUTOTRANSFUSION TRIPLE BAGS, W/O FILTERS AND KITS

☐ B0101010299 AUTOTRANSFUSION BAGS, W/O FILTERS AND KITS - OTHER

B0101010101: AUTOTRANSFUSION DOUBLE BAGS, WITH FILTERS AND KITS: Active			
Version	From	Action	Term
2	2025-10-31	Scope reduced	AUTOTRANSFUSION DOUBLE BAGS, WITH FILTERS AND KITS
1	2025-01-01	Inserted	AUTOTRANSFUSION DOUBLE BAGS, WITH FILTERS AND KITS

How does an EMDN code update affect my device?

1. If an EMDN code gets *scope-extended* or *corrected*, the device entry is not affected and no action is necessary.

Playground

Find the code Close

EMDN Code: EMDN Description:

Nomenclature already selected

L02 SUTURE INSTRUMENTS, REUSABLE

L0201 NEEDLES AND APPLICATORS FOR LIGATURES, REUSABLE i

☐ L020101 NEED ARMEN 1

☐ L020102 NEED ARMEN 2

☐ L020103 NEED ARMEN 3

☐ L020104 NEED ARMEN 4

☐ L0202 SUTURE NEEDLES, REUSABLE i

☐ L0203 SUTURE NEEDLES, REUSABLE - OTHER

L0204 SUTURE NEEDLES, REUSABLE

L0205 SUTURE NEEDLES, REUSABLE - OTHER

☐ L020501 NEEDLE HOLDER ARMEN 1

☐ L020502 NEEDLE HOLDER ARMEN 2 - CORRECTED i

☐ L0206 GROOVED PROBES, REUSABLE

☐ L0207 KNOT PUSHERS, REUSABLE

L0208 MULTIPLE CLIPS APPLICATORS, REUSABLE

☐ L020801 MULTIPLE CLIPS APPLICATORS FOR OPEN SURGERY, REUSABLE

☐ L020802 MULTIPLE APPLICATORS OF CLIPS FOR VIDEO SURGERY, REUSABLE

☐ L0299 SUTURE INSTRUMENTS, REUSABLE - OTHER

L0202: SUTURE NEEDLES, REUSABLE: Active

Version	From	Action	Term
2	2025-10-31	Scope extended	SUTURE NEEDLES, REUSABLE
1	2025-01-01	Inserted	SUTURE NEEDLES, REUSABLE

2. If an EMDN code gets *discarded* (inactive status), *split* or *scope-reduced*, the system will issue a warning (UDI details section):

UDI-DI 2222218932755260 See UDI-DI(s) list (1)

UDI-DI details

Version 2 [Draft] | Last update date: 2025-11-03

UDI-DI code: 2222218932755260

Issuing Entity: HIBCC

UDI-DI from another entity

UDI-DI from another entity (secondary) applicable: Yes

Secondary UDI-DI code: 22222189327552602

Issuing Entity: IFA

Selected nomenclature codes

Code L0204 STAPLE REMOVERS, REUSABLE

WARNING
Discarded (as of 2025-10-31)

Depending on the specific case, the system may prompt the user to remove the obsolete EMDN code before creating a new device version with the correct EMDN code. In such cases, the user will receive EUDAMED and email notifications.

EUDAMED Notification

Showing 1 to 3 of 3 entries Time received 11

Action 2025-11-07 | Email

UDI/Device - UDID-027: Change of EMDN code version

Due to a new version of the EMDN that has been entered in EUDAMED, it has been identified that your Actor DE-MF-000001601 - Fahey Group could need to create a new version of some of your device(s) to change their assigned EMDN code(s).

For EMDN code(s) 'Discarded' and 'Split', the change is mandatory, while for 'Reduced scope' it can be if the term description would not cover your device anymore.

The following EMDN code(s) assigned to your device(s) have been discarded:
L0204 - STAPLE REMOVERS, REUSABLE

The following EMDN code(s) assigned to your device(s) have been split:
L0201 - NEEDLES AND APPLICATORS FOR LIGATURES, REUSABLE, L0205 - NEEDLE HOLDERS, REUSABLE

The following EMDN code(s) assigned to your device(s) have their term description changed that reduces their scope:
L0203 - NEEDLE CONTAINERS, REUSABLE

Email Notification

 **MDR Eudamed**

UDID-027: Change of EMDN code version

Due to a new version of the EMDN that has been entered in EUDAMED, it has been identified that your Actor BE-MF-000001841 - EuMF-NECULA could need to create a new version of some of your device(s) to change their assigned EMDN code(s).

For EMDN code(s) 'Discarded' and 'Split', the change is mandatory, while for 'Reduced scope' it can be if the term description would not cover your device anymore.

The following EMDN code(s) assigned to your device(s) have been discarded:
Z11010101 - SINGLE ENERGY LINEAR ACCELERATORS - ARMEN REDUCED

CNS (Corporate Notification System)
[You can change your notification preferences here.](#)

- If applicable, enter the trade name (as specified on the device label) and select its related language (select **All languages** if not language-dependent):

Trade name applicable

Yes ☒ No ☐ Trade name is required unless you select the option - No

* Trade name:

* Select the language:

[+ Add a trade name in another language](#)

- Enter the *Reference/Catalogue number*.

* Reference/Catalogue number:

**NOTE**

For a Master UDI-DI, if there are multiple Reference/Catalogue numbers, you may enter "**many**" as the value:

Reference/Catalogue number

i If you have more than one Reference/Catalogue number, please enter the word 'many'

* Reference/Catalogue number:

many

6. Specify whether the device is directly marked or not:
- If the device is directly marked, you must either indicate it is the same as the UDI-DI or enter the UDI-DI and issuing entity of the Direct marking DI.

* Is the device directly marked?

☒ Yes ☐ No

☐ Same as UDI-DI

* Issuing Entity:

* Direct marking DI:

**NOTE**

Direct Marking UDI-DI is not applicable for a Master UDI-DI. The field is set to *No* and it is greyed out.

7. If the device is not directly marked and the base quantity of the device is **greater than one**, you may enter the Unit of Use DI and its issuing entity:
- The same Unit of Use DI (UoU DI) can be used for different UDI-DIs in case several units of the same device have different root packaging (each one having a different UDI-DI).

* Is the device directly marked?

☐ Yes ☒ No

* Quantity of device:

Issuing Entity:

Unit of Use DI:

**NOTE**

The *Unit of Use DI* and its *Issuing Entity* fields are not applicable for a Master UDI-DI. They are set to *No* and they are greyed out.

8. If the base quantity is **less than two**, then no Unit of Use DI (UoU DI) is provided:

* Is the device directly marked?

☐ Yes ☒ No

* Quantity of device:

1

* Type of UDI-PI

☐ Lot or Batch number

☐ Serial number

☐ Manufacturing date

☐ Expiration date

**NOTE**

For a Master UDI-DI, please indicate the maximum number of devices for the *Quantity of Device*:

Quantity of device

 Please indicate the maximum number of devices.

* Quantity of device:

20

9. Select the *Type of UDI-PI*. The UDI-PI is the production identifier for each unit. The different types of UDI-PIs include serial number, lot number, software identification and manufacturing or expiry date or both types of date, depending on how the device is produced.
10. Enter any additional pertinent information about the device, select the language in which the additional information is provided and enter a URL (web address) for additional information online if applicable:

Additional product description:

Product Description

 [Add additional product description in another language](#)

Select the language:

—

Bulgarian

Croatian

Czech

Danish

Dutch

English

URL for additional information (as electronic instructions for use):

11. Specify the status of the device by selecting whether it is *On the EU market*, *Not intended for the EU market* or *No longer placed on the EU market* and click **Save** or **Save & Next**:

*** UDI-DI status**

☐ No longer placed on the EU market
☒ Not intended for the EU market
☐ On the EU market

**NOTE**

A device *not intended for the EU market* may also be registered in EUDAMED.

3.1.4 Step 4: Enter UDI-DI characteristics

- Specify clinical size for the device if applicable and choose the dimension and the precision values in the drop-down lists below:

**NOTE**

When the selected *Clinical size* type has the option *Other*, users will be required to enter the *Description of the Clinical size type* and the language of description. The same applies for Measure unit.

In case both the Clinical size and Measure unit have the option *Other*, the description for the two fields needs to be provided in the same languages.

Clinical size applicable

Yes ☒ No ☐ Clinical size is required unless you select the option - No

Select type(s) of dimension you need

* Type:

* Precision: * Minimum: * Maximum: * Measure unit:

[Add a type of dimension](#)

You must provide one of the following precision types:

- Range – requires minimum and maximum values and the measure unit
- Text – requires free text entry
- Value – requires the size and the measuring unit


You may add several clinical sizes by adding different types of dimensions, but only one dimension for a given type.

2. Specify if the device is labelled as *single use*.

Single use device

When the device is not labelled *single use* you must provide the number of reuses if applicable:

- If the *Maximum number of reuses* is not applicable, then the device is considered as *non-single use Device* and it does not have a maximum number of reuses (infinite number of reuses)
- If value provided is ≥ 1 , the device is considered as a *non-single use Device* having a limited number of reuses (the value provided)

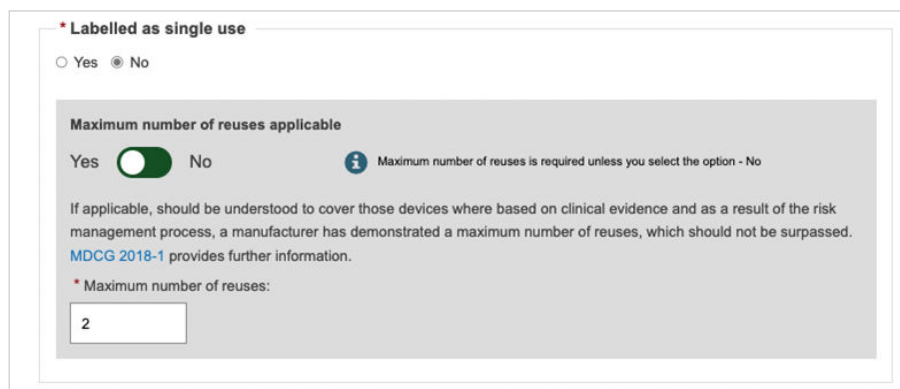

3. Select **Yes** or **No** for each of the options below:




NOTE

Containing latex is only for MDR, not applicable for IVDR.

4. For MDR devices, enter the information on whether the device contains any substance which could be CMR (carcinogenic, mutagenic, or toxic for reproduction) and/or Endocrine disruptor substances if applicable. When specifying CMR and/or Endocrine disruptor substances you may provide the EC# or CAS#. If you do provide them, only the *Name of substance* is required (the language is no longer required):

*** CMR/Endocrine disruptor**
 Labelled for presence of Carcinogenic, Mutagenic and toxic to Reproduction (CMR) substances of category 1A or 1B:

☒ Yes ☐ No

*** Category of CMR:**
☒ 1A ☐ 1B

At least one of these fields (EC# or CAS#) must be filled in.

EC#: CAS#:

[ECHA database >](#)

*** Name of the substance:**

[Add a CMR substance](#)

Labelled for presence of substance(s) with endocrine-disrupting properties:
☐ Yes ☐ No

5. Fill in the *Storage/handling conditions* section:

Storage/handling conditions, if applicable

Yes ☒ No ☐ Storage/handling conditions are required unless you select the option - No

*** Storage/handling conditions type:**

Description:

[Add another storage/handling condition](#)



NOTE

For Storage/handling conditions type *Other*, users must enter the Description of the *Storage/handling condition type* and the description's language.

6. Fill in *Critical warnings or contra-indications*, and click **Save** or **Save & Next**:

Critical warnings or contra-indications, if applicable

Yes ☒ No ☐ Critical warning or contra-indications are required unless you select the option - No

*** Critical warning type:**

*** Description:**

[Add critical warnings or contra-indications](#)

**NOTE**

For Critical warning or contra-indications type *Other*, users must enter the Description of the Critical warning or contra-indications *type* and the description's language.

3.1.5 Step 5: Enter additional device information

1. For MDR, specify if it is a reprocessed single use device and if it has an intended purpose other than medical (Annex XVI):

Device information

* Reprocessed single use device

☐ Yes ☐ No

* Intended purpose other than medical (Annex XVI)

☐ Yes ☐ No

2. If you select *Yes* for the *Intended purpose*, select the relevant purpose(s):

* Intended purpose other than medical (Annex XVI)

☒ Yes ☐ No

☒ Contact lenses

☒ Products intended to be totally or partially introduced in the human body

☐ Substances, combinations of substances, or items intended for filling by injection

☐ Equipment intended to be used to reduce, remove or destroy adipose tissue

☐ High intensity electromagnetic radiation

☐ Brain electrostimulation

**NOTE**

When registering a Master UDI-DI for contact lenses, if you select *Yes* for Annex XVI, the list of possible choices will not be displayed, as it is already predefined.

3. The (legal) manufacturer may use another natural or legal person(s) for design and manufacturing activities. However, the (legal) manufacturer, as defined by MDR and IVDR always bears the sole responsibility for device compliance.
Select **Yes** or **No** if the device was designed and manufactured by another legal or natural person.
If *Yes*, there are two ways to find the *Product original manufacturer* of the device:
 - Check the box *I know the Actor ID/SRN*, enter the Actor ID/SRN or name of the *Product original manufacturer* of the device and click **Check registry**:

Is the device designed and manufactured by another legal or natural person?

Yes ☒ No ☐

☒ I know the Actor ID/SRN

* Enter Actor ID/SRN or name:

**NOTE**

Check the box *I know the Actor ID/SRN* in order to search for an existing registered Manufacturer Actor either by SRN or by name.

Select the Actor from the list:

[Close](#)

Select manufacturer

Actor ID/SRN ↑↓	Organisation name ↑↓
NL-MF-000000041	Medical Device Manufacturer
AU-MF-000004268	Trusted NonEUMF
AS-MF-000004249	Non_EU_MF_R3.3_Shriya
BE-MF-000004247	Bel_MF_R3.3_Shriya
US-MF-000003888	The Americans
US-MF-000004107	Ohio Pharmaceuticals
CO-MF-000004129	Non_EU_MF_3.2_Shriya
BE-MF-000004128	MF_BE_R3.2_Shriya
EL-MF-000004067	VIANEX S.A.
AI-MF-000004047	AR Aguilla Ionut 2nd

1 2 ... 19

- Enter the name of the *Product original manufacturer organisation name* and click on **Check registry**:

Is the device designed and manufactured by another legal or natural person?

Yes ☒ No

☐ I know the Actor ID/SRN

* Product original manufacturer organisation name:

[Check registry](#)

Select the Organisation name from the list:

[Close](#)

Select manufacturer

Organisation name **!**

- PDasOrg (3)
- PDasOrg (2)
- MANUF-1(1)

i Select the relevant result above. If there are no results or they are not applicable, please select the option 'Enter data manually'

[Enter data manually](#) [Cancel](#)

If the Organisation name is not on the list, click on **Enter data manually** and fill in the required fields with the details on the *Product original manufacturer* of the device:

Playground

The screenshot shows a registration form for a manufacturer. At the top right, there is a link "Change manufacturer". The form fields are as follows:

- * Name (Manufacturer Name): A text box containing "PoMasOrg".
- Street information, if applicable: A toggle switch is set to "Yes". An information icon indicates "Street information is required unless you select the option - No".
- * Street: A text box containing "Via de Rosso".
- Street number: A text box containing "10".
- Address line 2: An empty text box.
- PO box: An empty text box.
- * City name: A text box containing "Milan".
- * Postal code: An empty text box.
- * Country: A dropdown menu showing "--".
- Telephone: An empty text box.
- Telephone format example: "+32 x xxx xx xx".
- * Email: An empty text box.

4. Select **Yes** or **No** to provide the Clinical Investigation/Performance study reference for the current device:

The screenshot shows the "Clinical Investigation / Performance Study" section. It includes a toggle switch set to "Yes" and an information icon stating "The information is required unless you select 'No'". Below this, there is a section titled "Clinical Investigation / Performance Study conducted inside EU?" with radio buttons for "Yes" and "No". At the bottom, there is a plus icon and a link "Add new Clinical Investigation / Performance Study".

5. When registering the devices under MDR, select **Yes** or **No** to fill information on tissues and cells, and information on substances:

*** Tissues and cells**

Presence of human tissues or cells, or their derivatives:

☐ Yes ☒ No

Presence of animal tissues or cells, or their derivatives:

☒ Yes ☐ No

Presence of cells or substances of microbial origin:

☐ Yes ☒ No

*** 'New' Device**

☒ Yes ☐ No 

If you answer **Yes** to Information on substances, enter the details:

*** Information on substances**

Presence of a substance which, if used separately, may be considered to be a medicinal product:

☒ Yes ☐ No

INN:

*** Name of the substance:**

*** Select the language:**

 [Add another language](#)

 [Add a substance](#)

Presence of a substance which, if used separately, may be considered to be a medicinal product derived from human blood or human plasma:

☐ Yes ☒ No

For IVDR, select **Yes** or **No** to fill information on tissues and cells and specify if the device is new.



NOTE

A device shall be considered **new** if:

- There has been no such device continuously available on the Union market during the previous three (3) years for the relevant analyte or other parameter.
- The procedure involves analytical technology not continuously used in connection with a given analyte or other parameter on the Union market during the previous three (3) years.

6. Choose a Member State in the dropdown list where the device is or has been first placed on the EU market, and click **Save** or **Save & Next**:

* Member State where the Device is to or has been first placed on the EU market:

France ▼

Member States where the device is or is to be made available on the market:

Finland	From			To			
		YYYY-MM-DD			YYYY-MM-DD		
France	From			To			
		YYYY-MM-DD			YYYY-MM-DD		

[Select one or more countries >](#)

**NOTE**

The countries where the device is or is to be made available on the market are mandatory, to be provided when the device's status is *On the EU market* and device's risk class is **not risk class I (MDR) and not risk class A (IVDR)**.

**NOTE**

It is possible to enter this information for all risk classes and this may be helpful for users searching for information on devices available in a particular MS.

3.1.6 Step 6: Enter container package details

**VIDEO: UDI carrier placing**

Please note that this video does not contain sound.



**NOTE**

Some devices may have more than one packaging level. In that case, each higher level of packaging shall have its own unique UDI. MDR and IVDR define packaging levels as the various levels of device packaging that contain a defined quantity of devices, such as a carton or case.

1. Click on *Add container package* when there is a higher packaging level for the root UDI-DI:

Each package level requires a unique UDI-DI assignment.

Start by registering the container package associated with the root UDI-DI (also known as the primary UDI-DI). You may add multiple levels and container packages. Input the *Issuing Entity*, UDI-DI code for the package, *Quantity per package*, select the *Package status* and then click **Save**:

**NOTE**

If the UDI-DI already exists in EUDAMED, the system will prevent you from saving.

**NOTE**

If the status of the device for this container package is either *No longer placed on the EU Market* or *Not intended for the EU Market*, the *Package status* options are greyed out and any container package added to this device will automatically have the same *Package status* as the device.

**NOTE**

When registering a Master UDI-DI code, a specific format validation algorithm is applied when the issuing entity is GS1:

- For **Standard soft contact lenses** and **Standard Rigid Gas Permeable (RGP) contact lenses** the system applies the GMN format validation algorithm.
- For **Made-to-order soft contact lenses** and **Made-to-order Rigid Gas Permeable (RGP) contact lenses** the system applies the GTIN format validation algorithm.

2. Select the generated information and click **Submit**:

Container package(s)

You are not obliged to provide container package(s) UDI-DI before submitting this request.

[Add container package](#)
[Edit container package](#)
[Delete container package](#)

☐ [Root] UDI-DI: product-original-manufacturer (ICCBBA) | Status: On the EU market

☒ UDI-DI: boxxx-6 (ICCBBA) | Quantity per package: 10 (10) | Status: On the EU market


Save

Submit >


Preview

3. Users with *Confirmer* profile can submit the device registration in the pop-up window. The device will be then registered and publicly available:

Playground

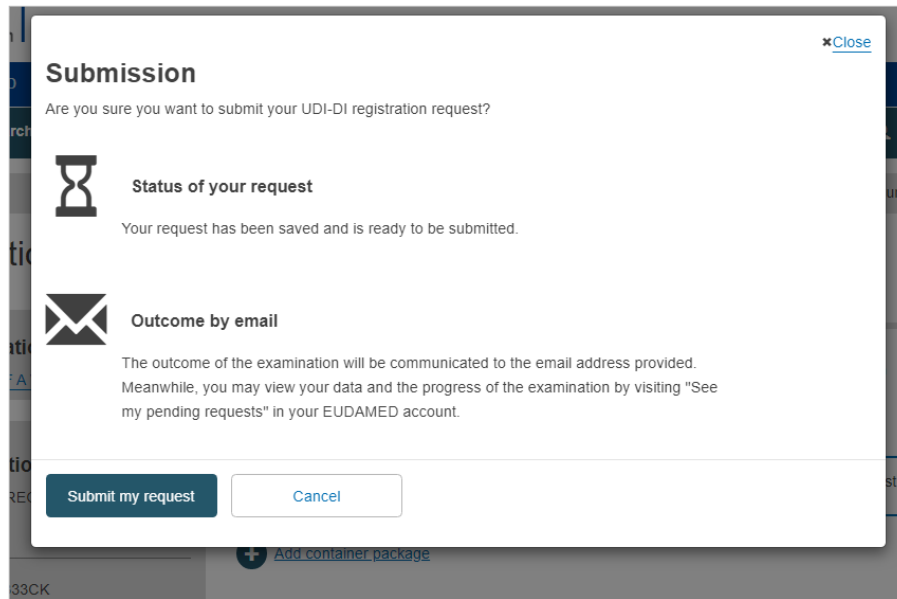

4. The screen will display a success message:

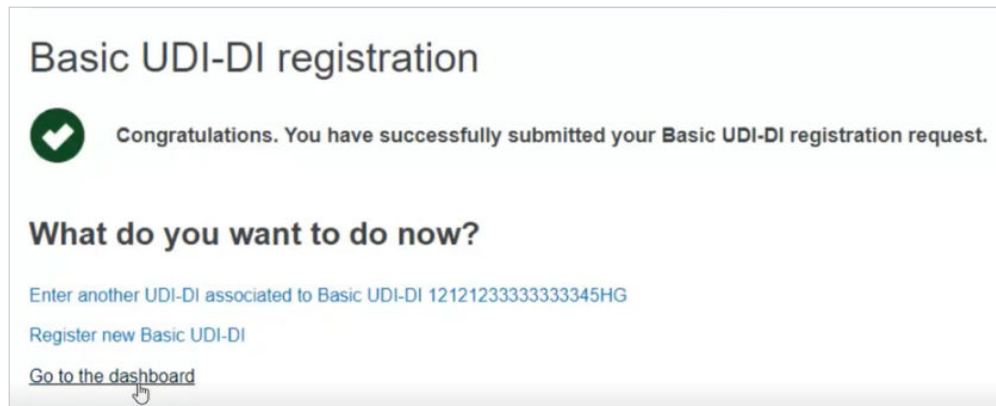

IMPORTANT

After submitting the Device, the state of the Device (Basic UDI-DI and UDI-DI) will be:

- **Registered**, if the Basic UDI-DI data does not require confirmation from the Notified Body (Basic UDI-DI and UDI-DI is publicly available in the EUDAMED public website);
- **Submitted**, if the Basic UDI-DI data requires confirmation from the Notified Body (Basic UDI-DI and UDI-DI is not publicly available and will only get the *Registered* state and become publicly available after Notified Body confirmation).

3.2 Register a regulation device and its UDI-DI for an existing Basic UDI-DI

1. On the EUDAMED Dashboard, select *Manage your Basic UDI-DIs/ EUDAMED DIs*:

Tasks

By module, consult, verify and/or manage your own and related data (managed by your actor), depending on your profile.

My Actor data

- Manage your actor data
- Manage your email notifications
- Machine to machine data delivery preferences

UDI-DIs/Device

- Register a new Basic UDI-DI
- Register a legacy device
- Manage your Basic UDI-DIs / EUDAMED DIs**
- Manage your device details

User management

- Assess user access requests
- Manage your users



NOTE

If you wish to register a regulation device, belonging to Basic UDI-DI already registered, the registration process is simplified, since some device details are already available in EUDAMED. Therefore, the registration starts by selecting the Basic UDI-DI.

- Filter the Basic UDI-DIs/ EUDAMED DIs in state *Submitted* or *Registered*:



IMPORTANT

Additional UDI-DIs for a Basic UDI-DI can be added only for Regulation Devices (not for Legacy Devices).

New devices and their UDI-DIs can be added only to Basic UDI-DIs that are in state *Registered* or *Submitted*:

Basic UDI-DIs / EUDAMED DIs management

Go to Device details management > Register a new Basic UDI-DI Register Legacy Device

Filter ▼

Applicable regulation

Risk class

State

Device type

Basic UDI-DI/EUDAMED DI Code

SRN AR

Apply filters Clear all filters

Active filters: State: Draft Clear all filters

Showing 1 to 12 of 12 entries Show 20 entries per page

Basic UDI-DI/EUDAMED DI Code	Devices	Device model	Device Name	Risk class	Date	State	Actions
122111212121Y2	1		Test	Class IIa	2021-03-31	1st Draft	...
1111184FG4G228694YC	1	DeviceModelZZZ	DeviceNameZZZ	Class IIb	2021-03-19	1st Draft	...

- From the results, find the Basic UDI-DI for which you wish to add a new device and its UDI-DI. Click on the three dots on the right and click on *Add a UDI-DI to this Basic UDI-DI* / *Add a Master UDI-DI to this Basic UDI-DI*:

Basic UDI-DIs / EUDAMED DIs management

[Go to Device details management](#) [Register a new Basic UDI-DI](#) [Register Legacy Device](#)

Filter

Active filters:
State: Registered [Clear all filters](#)

Showing 1 to 20 of 21 entries Show 20 entries per page

Basic UDI-DI/EUDAMED DI Code	Devices	Device model	Device Name	Risk class	Date	State	Actions
1234503276	1	Model OP		Class IIb	2021-03-30	Registered	...
1234503072	1	Model 88		Class IIb	2021-03-30		View Data
1234501VP	1	Model 1	Name 1A	Class III	2021-03-30		View all UDI-DIs for this Basic UDI-DI
B-555908900698	1	MyModel111	MyDeviceName111	Class I	2021-03-30		Add a UDI-DI to this Basic UDI-DI
1234500VM	1	Model 550		Class IIa	2021-03-08	Registered	...
123450046Z	2	Model 9		Class IIb	2021-03-08	Registered	...
B-2203615490541	1	Model abc	Name abc	Class IIa	2021-03-04	Registered	...

4. Complete the steps required for the registration of a UDI-DI for an existing Basic UDI-DI (*Step 3: UDI-DI identification information* [12], *Step 4: UDI-DI Characteristics* [21], *Step 5: Device information* [24], *Step 6: Container Package Details* [29]):

Add new UDI-DI to existing Basic UDI

Manufacturer identification
[BE-MF-000000004, Alexandru Release Manufacturer](#)

Basic UDI-DI identification
Applicable regulation: MDR (REGULATION (EU) 2017/745 on medical devices)
Basic UDI-DI code: 1234503276
Issuing Entity: GS1
Is it a System or Procedure Pack which is a Device in itself?
No
Special device type: No

1 UDI-DI identification information

2 UDI-DI characteristics

3 Device information

4 Container package(s)

UDI-DI identification

UDI-DI identification


* Issuing Entity: GS1 * UDI-DI code:

UDI-DI from another entity (secondary) applicable
Yes ☐ No ☒ UDI-DI from another entity is required unless you select the option - No

* Enter a nomenclature code (EMDN code):

[Advanced search of device nomenclature](#)

5. When you have completed all steps, click **Submit my request** to submit the new device registration request:

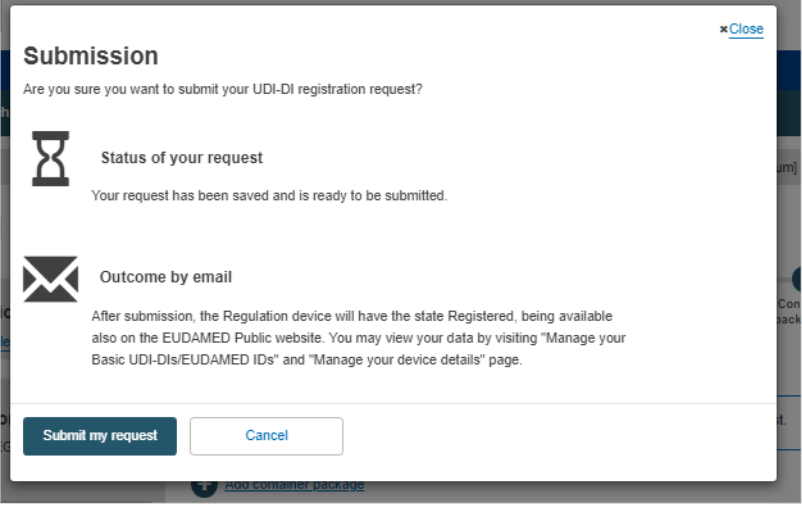

The screenshot shows a modal dialog titled "Submission" with a "Close" button in the top right corner. The dialog contains the following text:

Are you sure you want to submit your UDI-DI registration request?

Status of your request
Your request has been saved and is ready to be submitted.

Outcome by email
After submission, the Regulation device will have the state *Registered*, being available also on the EUDAMED Public website. You may view your data by visiting "Manage your Basic UDIs/EUDAMED IDs" and "Manage your device details" page.

At the bottom, there are two buttons: "Submit my request" (in a dark blue box) and "Cancel" (in a white box with a blue border).

**IMPORTANT**

After Submitting the device registration request, its state will be:

- **Registered** if the Basic UDI-DI has the state *Registered*;
- **Submitted** if the Basic UDI-DI has the state *Submitted*.

Playground

4 Register System or Procedure Packs (SPP)

4.1 Register Basic UDI-DI together with a UDI-DI for a System or Procedure Pack

Registering System or Procedure Packs is only possible for users belonging to an actor that is a System and Procedure Pack producer.

4.1.1 Step 1: Enter SPP and Basic UDI-DI main information

1. On the EUDAMED dashboard, click on *Register a New System Procedure Pack*:

Tasks

By module, consult, verify and/or manage your own and related data (managed by your actor), depending on your profile.

System or Procedure Pack

[Register a new System Procedure Pack](#)

[Manage your Basic UDI-DIs](#)

[Manage your UDI-DIs](#)

2. Next, specify the *Issuing Entity* and the *Basic UDI-DI code*:

System or Procedure Pack registration

Procedure pack producer identification

Organisation name:	AR_SPPP
SRN:	BE-PR-000000062
Address:	8686 Brussels
Telephone number:	-
Email:	ar_sppp@abc.com

Applicable regulation

MDR (REGULATION (EU) 2017/745 on medical devices)

Basic UDI-DI main information

* Issuing Entity:

--

* Basic UDI-DI code:

* System or Procedure Pack type:

☐ Procedure Pack
☐ System

Save & Next >



NOTE

Only legislation MDR (Regulation (EU) 2017/745 on medical devices) is possible for system and procedure packs (selected by default).

**IMPORTANT**

EUDAMED will validate the Basic UDI-DI code you insert based on the specific format provided by each Issuing Entity. Please ensure that you enter the correct code with the check digits. However, EUDAMED cannot verify that the code is correct beyond the format.

If the *Basic UDI-DI code* already exists in EUDAMED, the system will prevent you from saving – a Basic UDI-DI must be unique:

- Choose if you are registering a system or procedure pack and click on **Save & Next** to save your registration as a draft and move on to the next steps:

4.1.2 Step 2: Basic UDI-DI information

Enter the Basic UDI-DI information:

Playground

System or Procedure Pack registration

Producer identification

[BE-PR-000000062_AR_SPPP](#)

Basic UDI-DI identification

Applicable regulation: MDR (REGULATION (EU) 2017/745 on medical devices)

Basic UDI-DI code: 12121121212DL

Issuing Entity: GS1

System or Procedure Pack type: Procedure Pack

1 Basic UDI-DI information

2 UDI-DI identification information

3 UDI-DI characteristics

4 Container package(s)

Basic UDI-DI information

* Risk class:

--

* Indication of medical purpose:

* Select the language:

--

+ Add another indication of medical purpose

Device model applicable

Yes ☒ No ☐ Device model is required by default unless you select the option - No

* Model:

Name:

Save Save & Next >

1. Choose a *Risk Class* from the drop-down (it must be the highest risk class of devices that are part of the system or procedure pack):

Producer identification

[BE-PR-000000062_AR_SPPP](#)

Basic UDI-DI identification

Applicable regulation: MDR (REGULATION (EU) 2017/745 on medical devices)

Basic UDI-DI code: 12121121212DL

Basic UDI-DI information

* Risk class:

--

* Indication of medical purpose:

* Select the language:

--

+ Add another indication of medical purpose

2. Fill in the indication of medical purpose and select the related language from the drop-down list.

2017/745 on medical devices)

Basic UDI-DI code: 12121121212DL

Issuing Entity: GS1

System or Procedure Pack type: Procedure Pack

--

* Indication of medical purpose:

* Select the language:

--

+ Add another indication of medical purpose

If you add the indication in multiple languages, click on *Add another indication of medical purpose* and select its language.

Select **Yes** or **No** if Device model is applicable and, if so, enter the Device model and a device name if there is one. Otherwise, enter only a Device name:


Device model applicable

Yes ☒ No ☐ Device model is required by default unless you select the option - No

* Model:

Name:

- Click **Save** to save your registration as a draft, or click **Save & Next** to save it as a draft and continue to the next steps:



4.1.3 Step 3: UDI-DI identification information

- Select the *Issuing Entity* from the drop-down and enter the UDI-DI code:




IMPORTANT

The UDI-DI code must be unique. If it already exists in EUDAMED, you will not be able to save.




NOTE

In case your chosen Issuing Entity is GS1, the UDI-DI code you enter must be a 14-digit code including the check digit that will be used by EUDAMED to validate the UDI-DI code. If your GS1 UDI-DI (GTIN code) is shorter than 14 digits (check digit included), when populating EUDAMED field please add leading zero(s) until you reach 14 digits.

For example:

- 000000nnnnnnnn (GTIN-8)
- 00nnnnnnnnnnnnnn (GTIN-12)
- 0nnnnnnnnnnnnnnn (GTIN-13)

- Enter the Secondary UDI-DI from a different Issuing Entity to the UDI-DI if applicable:

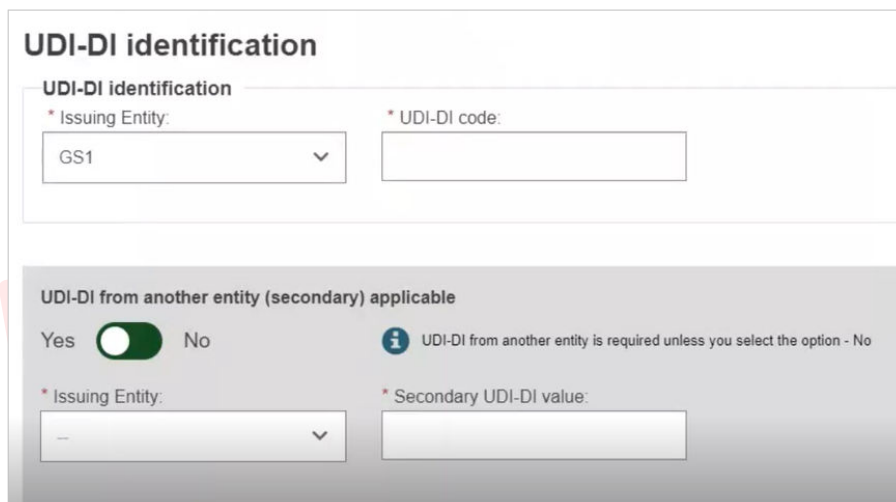

3. Enter the EMDN code, click **Find** and select the correct one from the list:

* Enter a nomenclature code (EMDN code):

 Find

[Advanced search of device nomenclature](#)

Selected nomenclature codes

[Code A0101010101](#) HYPODERMIC SYRINGE NEEDLES, WITH SAFETY SYSTEMS  [Remove nomenclature code](#)

Playground

**NOTE****Search for Nomenclature codes (EMDN)**

Click on **Advanced search of device nomenclature** to search by partial code name and view the list of codes alphabetically:

Find the code ✕ Close

EMDN Code: EMDN Description: Find

A DEVICES FOR ADMINISTRATION, WITHDRAWAL AND COLLECTION

A01 NEEDLES

A0101 NEEDLES FOR INFUSION AND SAMPLING

A010101 HYPODERMIC NEEDLES

A01010101 HYPODERMIC SYRINGE NEEDLES

☐ A0101010101 HYPODERMIC SYRINGE NEEDLES, WITH SAFETY SYSTEMS

☐ A0101010102 HYPODERMIC SYRINGE NEEDLES, W/O SAFETY SYSTEMS

A01010102 HYPODERMIC PEN NEEDLES

☐ A0101010201 HYPODERMIC PEN NEEDLES, WITH SAFETY SYSTEMS

☐ A0101010202 HYPODERMIC PEN NEEDLES, W/O SAFETY SYSTEMS

☐ A01010199 HYPODERMIC NEEDLES - OTHER

Confirm Cancel

EMDN Code updates

EMDN codes may get updated and therefore have a version history, which is indicated by an *information* icon.

Click on the *information* icon to view details about a code's versions and status:

Playground

UDI-DI from another entity (secondary) applicable

Find the code

EMDN Code: EMDN Description:

Nomenclature already selected

B010101 AUTOLOGOUS BLOOD COLLECTION BAGS

B01010101 AUTOTRANSFUSION BAGS, WITH FILTERS AND KITS

☐ B0101010101 AUTOTRANSFUSION DOUBLE BAGS, WITH FILTERS AND KITS i

☐ B0101010199 AUTOTRANSFUSION BAGS, WITH FILTERS AND KITS

B01010102 AUTOTRANSFUSION BAGS, WITH FILTERS AND KITS

☐ B0101010201 AUTOTRANSFUSION BAGS, WITH FILTERS AND KITS

☐ B0101010202 AUTOTRANSFUSION DOUBLE BAGS, W/O FILTERS AND KITS

☐ B0101010203 AUTOTRANSFUSION TRIPLE BAGS, W/O FILTERS AND KITS

☐ B0101010299 AUTOTRANSFUSION BAGS, W/O FILTERS AND KITS - OTHER

Version	From	Action	Term
2	2025-10-31	Scope reduced	AUTOTRANSFUSION DOUBLE BAGS, WITH FILTERS AND KITS
1	2025-01-01	Inserted	AUTOTRANSFUSION DOUBLE BAGS, WITH FILTERS AND KITS

How does an EMDN code update affect my device?

1. If an EMDN code gets *scope-extended* or *corrected*, the device entry is not affected and no action is necessary.

Playground

Find the code Close

EMDN Code: EMDN Description:

Nomenclature already selected

L02 SUTURE INSTRUMENTS, REUSABLE

L0201 NEEDLES AND APPLICATORS FOR LIGATURES, REUSABLE i

☐ L020101 NEED ARMEN 1

☐ L020102 NEED ARMEN 2

☐ L020103 NEED ARMEN 3

☐ L020104 NEED ARMEN 4

☐ L0202 SUTURE NEEDLES, REUSABLE i

☐ L0203 SUTURE NEEDLES, REUSABLE - OTHER

L0204 SUTURE NEEDLES, REUSABLE

L0205 SUTURE NEEDLES, REUSABLE - OTHER

☐ L020501 NEEDLE HOLDER ARMEN 1

☐ L020502 NEEDLE HOLDER ARMEN 2 - CORRECTED i

☐ L0206 GROOVED PROBES, REUSABLE

☐ L0207 KNOT PUSHERS, REUSABLE

L0208 MULTIPLE CLIPS APPLICATORS, REUSABLE

☐ L020801 MULTIPLE CLIPS APPLICATORS FOR OPEN SURGERY, REUSABLE

☐ L020802 MULTIPLE APPLICATORS OF CLIPS FOR VIDEO SURGERY, REUSABLE

☐ L0299 SUTURE INSTRUMENTS, REUSABLE - OTHER

L0202: SUTURE NEEDLES, REUSABLE: Active

Version	From	Action	Term
2	2025-10-31	Scope extended	SUTURE NEEDLES, REUSABLE
1	2025-01-01	Inserted	SUTURE NEEDLES, REUSABLE

2. If an EMDN code gets *discarded* (inactive status), *split* or *scope-reduced*, the system will issue a warning (UDI details section):

UDI-DI 2222218932755260 See UDI-DI(s) list (1)

UDI-DI details EDIT Delete

Version 2 [Draft] | Last update date: 2025-11-03

UDI-DI code: 2222218932755260

Issuing Entity: HIBCC

UDI-DI from another entity

UDI-DI from another entity (secondary) applicable: Yes

Secondary UDI-DI code: 22222189327552602

Issuing Entity: IFA

Selected nomenclature codes

Code L0204 STAPLE REMOVERS, REUSABLE

WARNING
Discarded (as of 2025-10-31)

Depending on the specific case, the system may prompt the user to remove the obsolete EMDN code before creating a new device version with the correct EMDN code. In such cases, the user will receive EUDAMED and email notifications.

EUDAMED Notification

Showing 1 to 3 of 3 entries Time received 11

Action 2025-11-07 | Email

UDI/Device - UDID-027: Change of EMDN code version

Due to a new version of the EMDN that has been entered in EUDAMED, it has been identified that your Actor DE-MF-000001601 - Fahey Group could need to create a new version of some of your device(s) to change their assigned EMDN code(s).

For EMDN code(s) 'Discarded' and 'Split', the change is mandatory, while for 'Reduced scope' it can be if the term description would not cover your device anymore.

The following EMDN code(s) assigned to your device(s) have been discarded:
L0204 - STAPLE REMOVERS, REUSABLE

The following EMDN code(s) assigned to your device(s) have been split:
L0201 - NEEDLES AND APPLICATORS FOR LIGATURES, REUSABLE, L0205 - NEEDLE HOLDERS, REUSABLE

The following EMDN code(s) assigned to your device(s) have their term description changed that reduces their scope:
L0203 - NEEDLE CONTAINERS, REUSABLE

Email Notification



European Commission

MDR Eudamed

UDID-027: Change of EMDN code version

Due to a new version of the EMDN that has been entered in EUDAMED, it has been identified that your Actor BE-MF-000001841 - EuMF-NECULA could need to create a new version of some of your device(s) to change their assigned EMDN code(s).

For EMDN code(s) 'Discarded' and 'Split', the change is mandatory, while for 'Reduced scope' it can be if the term description would not cover your device anymore.

The following EMDN code(s) assigned to your device(s) have been discarded:
Z11010101 - SINGLE ENERGY LINEAR ACCELERATORS - ARMEN REDUCED

CNS (Corporate Notification System)
[You can change your notification preferences here.](#)

4. If applicable, enter the trade name (as specified on the device label) and select its related language (select **All languages** if not language dependent):

Trade name applicable

Yes ☒ No ☐ Trade name is required unless you select the option - No

* Trade name:

* Select the language:

—
I
▼

+ [Add a trade name in another language](#)

5. Enter the *Reference/Catalogue number*.
6. Select the *Type of UDI-PI*.
7. Enter any additional pertinent information about the System or Procedure Pack, select the language of the additional information and enter a URL (web address) for additional information online, if applicable:

Additional product description:

Product Description

Select the language:

Bulgarian
Croatian
Czech
Danish
Dutch
English

+ Add additional product description in another language

URL for additional information (as electronic instructions for use):

- Specify the *UDI-DI status* in selecting whether it is *On the EU market*, *Not intended for the EU market* or *No longer placed on the EU market* and click **Save** or **Save & Next**:

* UDI-DI status

☐ No longer placed on the EU market

☒ Not intended for the EU market

☐ On the EU market

Save Save & Next >

4.1.4 Step 4: UDI-DI characteristics

- Select Yes or No for each option regarding sterilisation:

Basic UDI-DI information UDI-DI identification information UDI-DI characteristics Container package(s)

UDI-DI characteristics

* Need for sterilisation before use

☐ Yes ☐ No

* Device labelled as sterile

☐ Yes ☐ No

- If Storage/handling conditions are applicable, slide the toggle to **Yes**. Choose the correct information from the list and provide a description where relevant:

Storage/handling conditions, if applicable

Yes ☒ No ☐ Storage/handling conditions are required unless you select the option - No

* Storage/handling conditions type:

OTHER *

* Description:

Test

* Select the language:

—

+ [Add storage/handling conditions in another language](#)

+ [Add another storage/handling condition](#)

**NOTE**

When the selected Storage/handling conditions type has the option *Other*, users will be required to enter the Description of the Storage/handling condition type and the description's language.

3. Do the same for Critical warnings or contra-indications, and click **Save** or **Save & Next**:

Critical warnings or contra-indications, if applicable

Yes ☒ No ☐ Critical warning or contra-indications are required unless you select the option - No

* Critical warning type:

Cautious: Contains of presence of...
Defibrillation-proof type CF applied part

* Description:

Test

+ [Add critical warnings or contra-indications](#)

Save Save & Next >

**NOTE**

When the selected Critical warning or contra-indications type has the option *Other*, users will be required to enter the Description of the Critical warning or contra-indications type and the description's language.


4. Click **Save** to save draft and finish later or **Save & Next** to move directly to the next step of the process:

Save Save & Next >

4.1.5 Step 5: Container package details

VIDEO: UDI and Systems and Procedure Packs

Please note that this video contains sound.

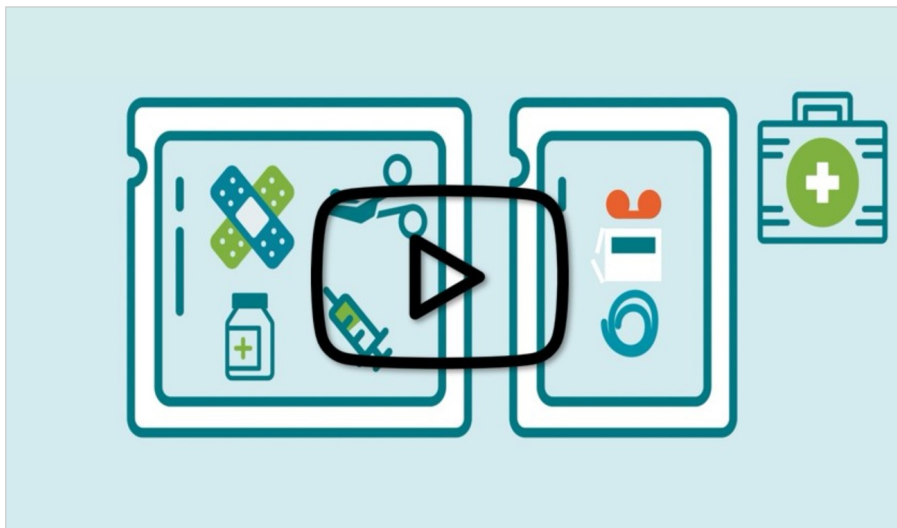

1. Click on *Add container package* when there is a higher packaging level for the root UDI-DI:

The screenshot shows a web interface with a light blue header bar containing an information icon and the text: "You are not obliged to provide container package(s) UDI-DI before submitting this request." Below this is a section with a plus icon and the text "Add container package". At the bottom of the section are three buttons: "Save", "Submit >", and "Preview".

A unique UDI-DI must be assigned to each package level. You add a higher container package to the root UDI-DI if there is no container package UDI-DI yet, or to the selected UDI-DI (you can add as many levels and as many container packages per level as you have). Add the *Issuing Entity*, *Package UDI-DI code* and the *Quantity per package*, select the *Package status* and click **Save**:



NOTE

If the UDI-DI already exists in EUDAMED, the system will prevent you from saving.

[*Close](#)

Add container package

 Container package UDI-DI for **UDI-DI product-original-manufacturer**

* Issuing Entity:	* Package UDI-DI code:	* Quantity per package:	Total number of devices
-		1	1

* Package status

☐ No longer placed on the EU market

☐ Not intended for EU market

☒ On the EU market

**NOTE**

If the status of the device for this container package is either *No longer placed on the EU Market* or *Not intended for the EU Market*, the *Package status* options are greyed out and any container package added to this device will automatically have the same *Package status* as the device.

2. Select the generated information and click on **Submit**:

Container package(s)


 You are not obliged to provide container package(s) UDI-DI before submitting this request.

 [Add container package](#)
 [Edit container package](#)
 [Delete container package](#)


- ☐ [Root] UDI-DI: product-original-manufacturer (ICCBBA) | Status: On the EU market

☒ UDI-DI: boxxx-6 (ICCBBA) | Quantity per package: 10 (10) | Status: On the EU market

3. On the pop-up window, click on **Submit my request**:

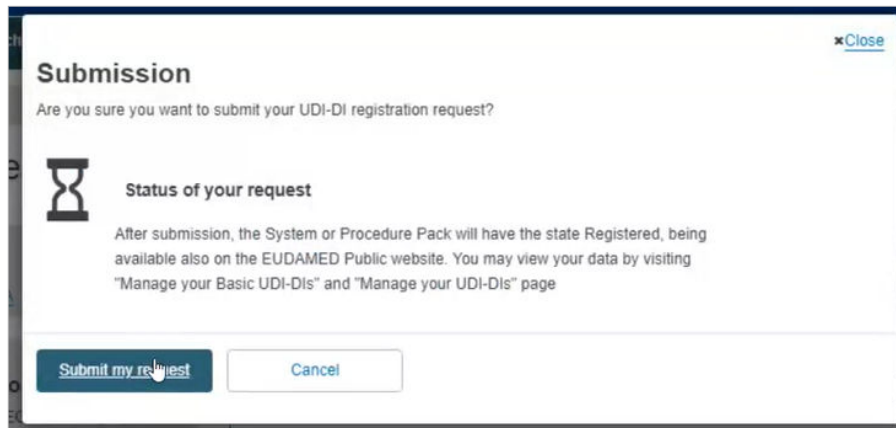


Upon submission, a success message will be displayed on the screen:

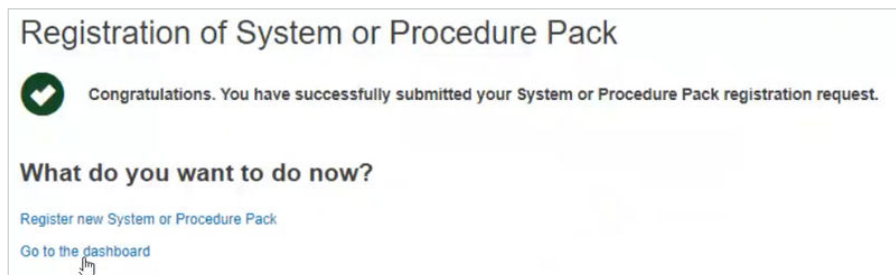

4.2 Register a new System or Procedure Pack UDI-DI for an existing Basic UDI-DI

1. On the Dashboard, select *Manage your Basic UDI-DIs*:

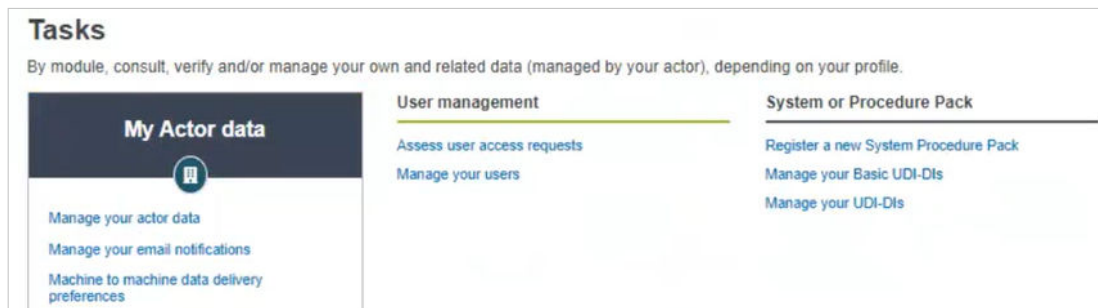

2. Filter the Basic UDI-DIs with the state *Registered*:
To do that click on the button **Filter**, then select *Registered* in the *State* box and then click on the button **Apply filters**:

Basic UDI-DI management for SPP

[Go to device management](#) [Register new System or Procedure Pack](#)

Filter ▼

Basic UDI-DI code: Name: State:

Risk class: System or Procedure Pack:

[Apply filters](#) [Clear all filters](#)

State dropdown menu:

- Draft
- Discarded
- Draft**
- Registered
- Submitted

New UDI-DIs can be added only for Basic UDI-DIs in state *Registered* or *Submitted*.

- Identify the Basic UDI-DI for which you would like to add a new UDI-DI and click on the ellipsis symbol to add it:

Basic UDI-DI code	UDI-DI(s)	Device model	Device Name	Risk class	Type	Date	State	Actions
1212112121212DL	1	-	Device Name	Class IIa	PP	2021-06-10	Registered	...
12345KT-Devices-3BY	1	-	test	Class I	PP	2021-05-2		View Data
223311445578899583F	1	SPP_Model		Class I	S	2021-04-0		View all UDI-DIs for this Basic UDI-DI

+

Add a UDI-DI for a Basic UDI-DI

4.2.1 Step 1: UDI-DI identification information

- Complete all the necessary information in the *UDI-DI identification information* tab:

Playground

1

UDI-DI identification information

2

UDI-DI characteristics

3

Container package(s)

UDI-DI identification

UDI-DI identification

* Issuing Entity:

HIBCC

* UDI-DI code:

121212

UDI-DI from another entity (secondary) applicable

Yes ☒ No

i

UDI-DI from another entity is required unless you select the option - No

* Enter a nomenclature code (EMDN code):

Find

[Advanced search of device nomenclature](#)

Selected nomenclature codes

Code A01010101 HYPODERMIC NEEDLES FOR SYRINGE

Remove nomenclature code

Trade name applicable

Yes ☒ No

i

Trade name is required unless you select the option - No

* Trade name:

Trade_Name

* Select the language:

Croatian

+ Add a trade name in another language

* Reference/Catalogue number:

Ref_12134

REF_TEST

Ref_12134

☐ Manufacturing date

☐ Expiration date

2. Click on **Save & Next** to move to the next step:

Save

Save & Next

4.2.2 Step 2: UDI-DI characteristics

1. Fill in the fields for the UDI-DI *Characteristics* tab:

UDI-DI characteristics

*** Need for sterilisation before use**

☐ Yes ☒ No

*** Device labelled as sterile**

☐ Yes ☒ No

Storage/handling conditions, if applicable

Yes ☒ No Storage/handling conditions are required unless you select the option - No

Critical warnings or contra-indications, if applicable

Yes ☒ No Critical warning or contra-indications are required unless unless you select the option - No

*** Critical warning type:**

Description

[Add critical warnings or contra-indications](#)

Save

Save & Next >

2. Click **Save & Next** to move directly to the next step (or click **Save** to save your draft for later).

4.2.3 Step 3: Container package details


To complete this step, please consult [Container Package Details \[47\]](#) of this guide.

Playground

5 Manage your Device information

5.1 Manage your device details and Basic UDI-DI/EUDAMED DI

- On the dashboard, click *Manage your Basic UDI-DI/EUDAMED DIs*:

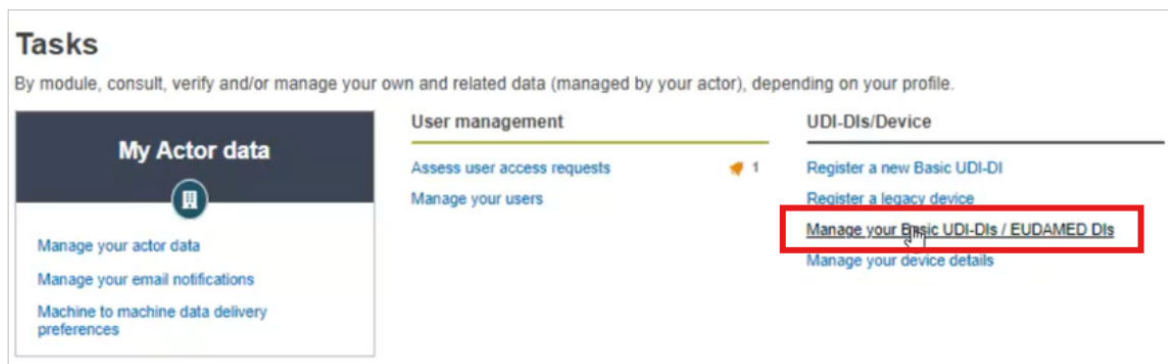

- You will see a list with all of the Basic UDI-DIs /EUDAMED DIs registered to the current actor:



NOTE

By default, the devices listed are the ones in *draft* state (not yet *submitted*, nor *registered*). To retrieve devices in other states, use the filters.

Basic UDI-DIs / EUDAMED DIs management

Go to Device details management > Register a new Basic UDI-DI Register Legacy Device

Filter ▼

Active filters: State: Draft Clear all filters

Showing 1 to 9 of 9 entries Show 20 entries per page

Basic UDI-DI/EUDAMED DI Code IT	Devices IT	Device model IT	Device Name IT	Risk class	Date IT	State	Actions
B-12121EL	1		Test	Class IIb	2021-04-01	1st Draft	...
12121212IU5	1		Test	Class IIa	2021-04-01	1st Draft	...
1211421211211EW	1		Device Name	Class IIa	2021-04-01	Draft	...
31212121121212133383	2	Device Model_Test_CLASS IIa_v3	Device Name	Class IIa	2021-03-16	Draft	...
12121233333333343HC	1		test	Class I	2021-02-15	1st Draft	...
12345ABCBY	1		test	Class I	2021-02-05	1st Draft	...

- Click on the three dots on the right of the desired entry and then click on *View Data* from the list:

Date ↑	State	Actions
2021-06-09	Draft	...
2021-		View Data
2021-		Edit Data
2021-		View all UDI-DIs for this Basic UDI-DI

- You will see a summary of the details concerning your device and its Basic UDI-DI/
EUDAMED DI:

CURRENT ACTOR: Manufacturer, FR-MF-000004867, Martin-Moreau & Fils. [France] [Notifications](#)

Basic UDI-DI 04072025TWDEMO-IVDR-AAH

[Go to Basic UDI-DI/EUDAMED DI management](#)

Basic UDI-DI details

UDI-DI(s) (1)

Basic UDI-DI details

Clinical Investigation / Performance Study

Version 1 [Current] | Last update date: 2025-07-03

Applicable regulation:

IVDR (REGULATION (EU) 2017/746 on in vitro diagnostic medical devices)

Basic UDI-DI code:

04072025TWDEMO-IVDR-AAH

Issuing Entity:

GS1

Kit:

No

Special device type:

No

Risk class:

Class A

Near-patient testing:

Yes

Self-patient testing:

No

Companion diagnostic:

No

Reagent:

No

Create new version

5.1.1 Delete draft Basic UDI-DI/EUDAMED DI

After following steps 1, 2 and 3 from [Manage your device Basic UDI-DI/EUDAMED DI details \[53\]](#) to view a Draft Basic UDI-DI/EUDAMED DI in state *1st draft*, you have the option to delete this draft.

- Inside the *View details* page of the desired 1st draft, click **Delete**:

Playground

CURRENT ACTOR: Manufacturer, FR-MF-000004867, Martin-Moreau & Fils. [France] [Notifications](#)

Basic UDI-DI 697901234567893M

[Go to Basic UDI-DI/EUDAMED DI management](#)

Basic UDI-DI details **UDI-DI(s) (0)**

Basic UDI-DI details

Clinical Investigation / Performance Study

Basic UDI-DI details [Edit](#) [Delete](#)

Version 1 [Draft] | Last update date: 2024-10-22

Applicable regulation:	MDR (REGULATION (EU) 2017/745 on medical devices)
Basic UDI-DI code:	697901234567893M
Issuing Entity:	GS1
Is it a System or Procedure Pack which is a Device in itself?:	No
Special device type:	No
Risk class:	Class I
Implantable:	No

- A pop-up window will ask you to confirm the deletion.
The system also warns about simultaneous deletion of any associated device *1st draft* UDIs:

Basic UDI-DI 189655498498748H

[Go to Basic UDI-DI/EUDAMED DI management](#)

Basic UDI-DI details **UDI-DI(s) (1)**

Basic UDI-DI details

Clinical Investigation / Performance Study

Delete Basic UDI-DI [Close](#)

Delete Basic UDI-DI and all its related elements? Basic UDI-DI has the following UDI-DI associated:

- 54687i6

Continue operation?

[Confirm](#) [Cancel](#)

Version 1 [Draft] | Last update date: 2025-05-02

Applicable regulation:	MDR (REGULATION (EU) 2017/745 on medical devices)
Basic UDI-DI code:	189655498498748H

5.1.2 Update (create new version of the record) for Basic UDI-DI/EUDAMED DI

Follow the steps in section [Manage your device Basic UDI-DI/EUDAMED DI details \[53\]](#) to view a device and its Basic UDI-DI/EUDAMED DI.

- Once inside the details page for the desired device and its Basic UDI-DI, click on **Create new version** on the top right corner:

Playground

CURRENT ACTOR: Manufacturer, FR-MF-000004867, Martin-Moreau & Fils. [France]  Notifications

Basic UDI-DI 04072025TWDEMO-IVDR-AAH

[Go to Basic UDI-DI/EUDAMED DI management](#)

Basic UDI-DI details UDI-DI(s) (1)

Basic UDI-DI details

[Clinical Investigation / Performance Study](#)

Version 1 [Current] | Last update date: 2025-07-03

[Create new version](#)

Applicable regulation:	IVDR (REGULATION (EU) 2017/746 on in vitro diagnostic medical devices)
Basic UDI-DI code:	04072025TWDEMO-IVDR-AAH
Issuing Entity:	GS1
Kit:	No
Special device type:	No
Risk class:	Class A
Near-patient testing:	Yes
Self-patient testing:	No
Companion diagnostic:	No
Reagent:	No

2. Update the desired details:

04072025TWDEMO-IVDR-AAH [version: 2]

Create a new version of 04072025TWDEMO-IVDR-AAH

Basic UDI-DI code:	04072025TWDEMO-IVDR-AAH
Issuing Agency:	GS1
Special device type:	No
Risk class:	Class A
Near-patient testing:	Yes
Self-patient testing:	No
Companion diagnostic:	No
Reagent:	No
Instrument:	No
Professional Testing:	No
Device model applicable	☒ Yes ☐ No  Device model applicable
* Device Name:	TW DEMO - IVDR Class A
Presence of human tissues or cells, or their derivatives:	No
Presence of animal tissues or cells, or their derivatives:	No
Presence of a substance which, if used separately, may be considered to be a medicinal product:	-
Presence of a substance which, if used separately, may be considered to be a medicinal product derived from human blood or human plasma:	-
Presence of cells or substances of microbial origin:	No

3. To complete the action:

- Click **Save** to save to your registration as a draft and continue later.
- Click **Submit new version** if you are certain about the update and wish to submit it.

Alternatively, click **Cancel** to cancel the update.

5.1.3 View historical versions of device data and its Basic UDI-DI/EUDAMED DI

Follow the steps in section [Manage your device Basic UDI-DI/EUDAMED DI details \[53\]](#) to view data on a device and its Basic UDI-DI/EUDAMED DI.

1. Once inside the details of the selected device and its Basic UDI-DI, click *See version history*:

Basic UDI-DI data

Version 4 [Current] | [See version history](#) | Last update date: 2021-06-10

[Create new version](#)

Applicable regulation:	MDR (REGULATION (EU) 2017/745 on medical devices)
Basic UDI-DI code:	12345-test-udi-1-HL
Issuing Entity:	GS1
Is it a System or Procedure Pack which is a Device in itself?:	Procedure Pack which is a device in itself

2. View the list of versions for the desired Basic UDI-DI and click on the version you wish to view:

Basic UDI-DI 12345-test-udi-1-HL

[Go back to the current version](#)

Version history of Basic UDI-DI 12345-test-udi-1-HL

Version 3 - Last update date: 2021-06-09	>
Version 2 - Last update date: 2021-06-09	>
Version 1 - Last update date: 2021-05-03	>

3. Inside a version, you can browse through the different versions by clicking on the arrows at the top right corner:

[Go back to the current version](#)

Version history of Basic UDI-DI 12345-test-udi-1-HL

See all version history (3) | [Previous version \[v1\]](#) | [Next version \[v3\]](#)

Version 2 - Last update date: 2021-06-09

Basic UDI-DI identification

Applicable regulation: MDR (REGULATION (EU) 2017/745 on medical devices)

Basic UDI-DI code: 12345-test-udi-1-HL

Issuing Entity: GS1

Is it a System or Procedure Pack which is a Device in itself? Procedure Pack which is a device in itself

Risk class: Class IIb

Implantable: No

5.2 Manage your device UDI-DI/EUDAMED ID details

- On the EUDAMED dashboard, click on *Manage your device details*:

Tasks

By module, consult, verify and/or manage your own and related data (managed by your actor), depending on your profile.

My Actor data

Manage your actor data

Manage your email notifications

Machine to machine data delivery preferences

UDI-DIs/Device

Register a new Basic UDI-DI

Register a legacy device

Manage your Basic UDI-DIs / EUDAMED DIs

Manage your device details

User management

Assess user access requests

Manage your users

- You will see a list:

Showing 1 to 20 of 50 entries


Show entries per page

(Master) UDI-DI/EUDAMED ID IT	Trade name IT	Reference/Catalogue number IT	Nomenclature code IT	Date IT	Status	State	Actions
Basic UDI-DI code: 12345-DDD-05-6Z, Device Model: AAA, Class IIb, MDR (REGULATION (EU) 2017/745 on medical devices)							
12311ss	AAA	099OPP		2024-06-25	On the EU market	1st Draft	...
EUDAMED DI code: B-nlkoIVD, Device Name: odjcouwbfk, Class I, MDD (Directive 93/42/EEC on Medical Devices)							
D-nlkoIVD				2024-06-25	On the EU market	1st Draft	...
Basic UDI-DI code: 888888888888BB, Device Model: test delete master UDI, Class I, MDR (REGULATION (EU) 2017/745 on medical devices)							
opo-91910	test delete master UDI	R0191		2024-06-25	On the EU market	Draft	...
EUDAMED DI code: B-ivdd+generalFA, Device Model: AAA, IVD Annex II List A, IVDD (Directive 98/79/EC on in vitro Diagnostic Medical Devices)							
D-ivdd+generalFA				2024-06-21	On the EU market	1st Draft	...
EUDAMED DI code: B-aimddP8, Device Model: SSw, AIMDD, AIMDD (Directive 90/385/EEC - Active Implantable Medical Devices)							
D-aimddP8				2024-06-21	On the EU market	1st Draft	...
EUDAMED DI code: B-mdd+cert6F, Device Model: ggg, Class III, MDD (Directive 93/42/EEC on Medical Devices)							
D-mdd+cert6F				2024-06-21	On the EU market	1st Draft	...
Basic UDI-DI code: 7777777777770UZ, Device Name: aaaaaaaaaa, Class I, MDR (REGULATION (EU) 2017/745 on medical devices)							
HIB-020nbf		q1211sdrw		2024-06-18	On the EU market	1st Draft	...
Basic UDI-DI code: 12345-master-udi-di-1-6C, Device Model: Master UDI-DI model, Class III, MDR (REGULATION (EU) 2017/745 on medical devices)							
12345756984101	sdsdfcd	as23r43x		2024-06-18	On the EU market	1st Draft	...

**NOTE**

By default, the system lists the devices in *draft* state. To retrieve other states use the filters:

3. Click on the three dots on the right of the desired entry and then *View data*:

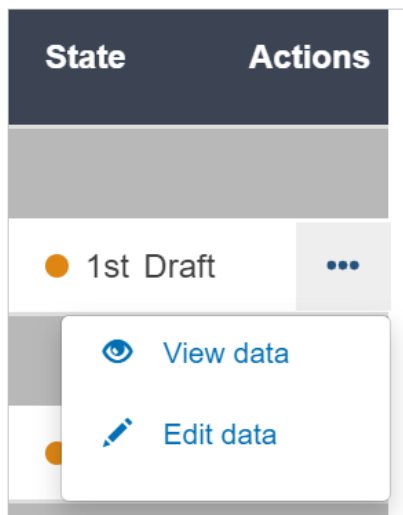

4. You will see a summary of the details of your device:

Playground

UDI-DI u-123123MI9N

See UDI-DI(s) list (1)

UDI-DI data

Product original manufacturer

Market Information

Container Package Information

UDI-DI data

Version 6 [Draft] | See version history | Last update date: 2023-09-15

UDI-DI code:

u-123123MI9N

Issuing Entity:

HIBCC

UDI-DI from another entity

UDI-DI from another entity (secondary) applicable:

No

Selected nomenclature codes

Code A01010101 HYPODERMIC SYRINGE NEEDLES, WITH SAFETY SYSTEMS

Trade name

Trade name applicable:

No

Reference/Catalogue number:

fghgf

Is the device directly marked?

Is the device directly marked?:

No

Quantity of device:

1

Type of UDI-PI

Lot or Batch number:

Yes

Additional product description:

gh [BG]

EDIT

DELETE

5.2.1 Delete draft UDI-DI/EUDAMED ID

Follow the steps in [Manage your device UDI-DI/EUDAMED ID details \[58\]](#) to view a draft UDI-DI.

- Once inside the desired device's Draft UDI-DI, click **Delete**:

Basic UDI-DI 189655498498748H

Go to Device Details management

Basic UDI-DI details

UDI-DI(s) (1)

UDI-DI 54687i6

See UDI-DI(s) list (1)

UDI-DI details

Product original manufacturer

Container Package Information

UDI-DI details

Version 1 [Draft] | Last update date: 2025-05-02

UDI-DI code:

54687i6

Issuing Entity:

HIBCC

UDI-DI from another entity

UDI-DI from another entity (secondary) applicable:

No


Selected nomenclature codes

Code T01010202 NITRILE SURGICAL GLOVES

EDIT


Delete

- A pop-up message will ask you to confirm the deletion.
The system will also warn about simultaneous deletion of the associated Basic UDI-DI, in case there is only this single device under it:

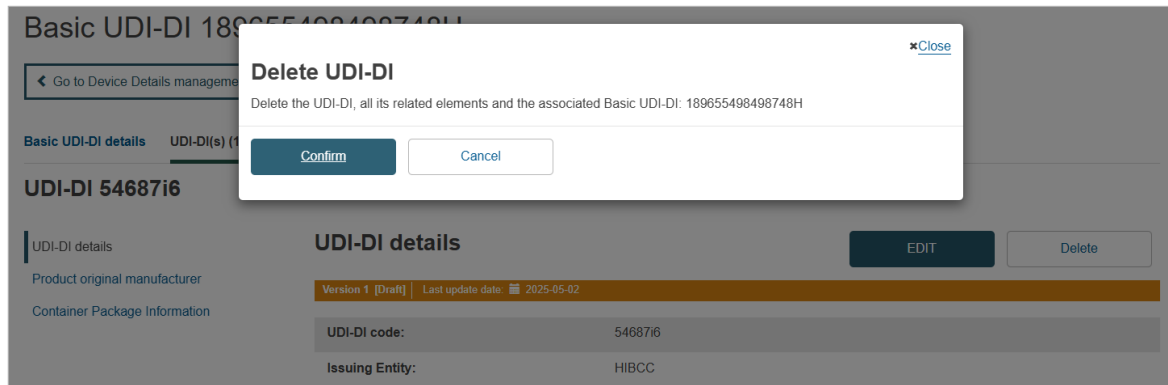


5.2.2 View details of a registered device and its UDI-DI/ EUDAMED ID details

1. On the dashboard, click *Manage your device details*:

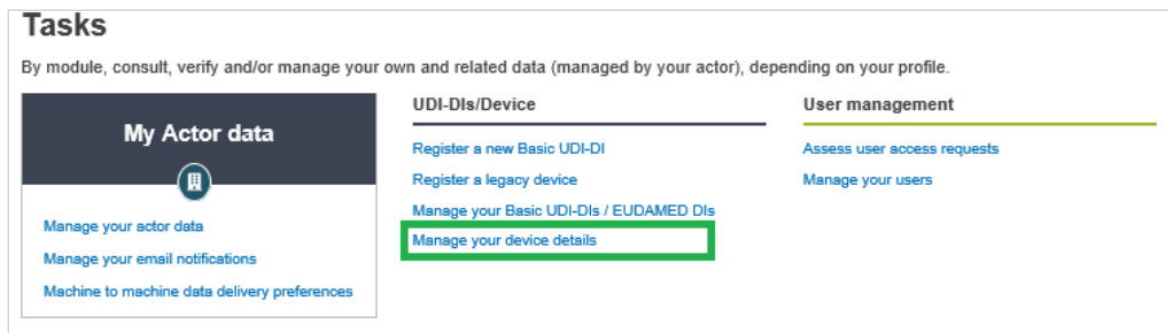

2. Select the option *Registered* in the *State* field and click **Apply filters**:

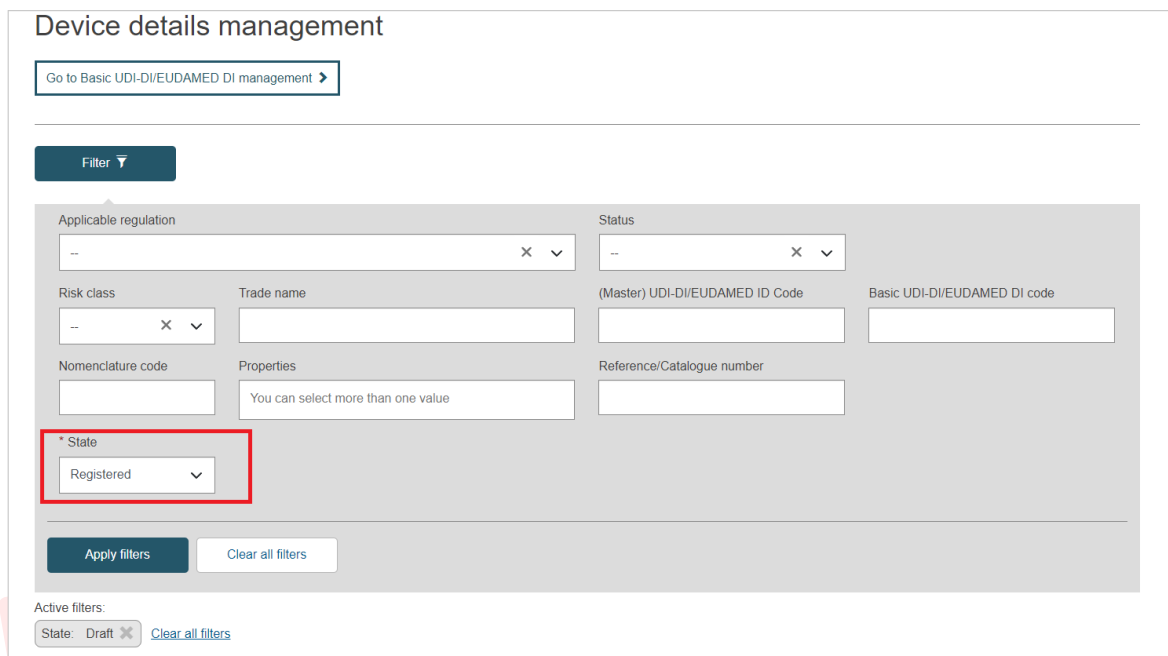

3. A list of devices will be displayed. Click *View data* under the three dots of the relevant entry:

Showing 1 to 20 of 454 entries

Show entries per page

UDI-DI/EUDAMED ID Code II	Trade name II	Reference/Catalogue number II	Nomenclature code II	Date II	Status	State	Actions
Basic UDI-DI code: 777777777770UZ, Device Name: aaaaaaaaaa, Class I, MDR (REGULATION (EU) 2017/745 on medical devices)							+ Add a new Master UDI-DI
188727_00	aaaaaaaaa	0101912		2024-06-17	On the EU market	Registered	...
Basic UDI-DI code: 109784903285972P5, Device Name: DV_NM-BRB, Class IIa, MDR (REGULATION (EU) 2017/745 on medical devices)							+ Add a new UDI-DI
BRB-cd-1		brb-dev-rn		2024-06-11	On the EU market	Registered	...
Basic UDI-DI code: 12345-24.Q1-Ilb-mfs-2-XU, Device Model: 12345-24.Q1-Ilb-mfs-2-XU, Class IIb, MDR (REGULATION (EU) 2017/745 on medical devices)							View data
brb-test-code		BRB-RN		2024-06-11	On the EU market	Registered	...
12345-24.Q1-Ilb-mfs-2-XU8	Generic Device Name_Device 1	12345-24.Q1-Ilb-mfs-2-XU		2024-06-03	On the EU market	Registered	...
Basic UDI-DI code: 12345-family-mudi-1-Q4, Device Model: My model, Class IIa, MDR (REGULATION (EU) 2017/745 on medical devices)							+ Add a new Master UDI-DI

4. You will see a summary of your device details, divided into the following subsections:
- UDI-DI details:

UDI-DI details

[Discard](#)[Create new version](#)

Version 1 [Current] | Last update date: 2024-06-20

UDI-DI code:

00125877641269

[Link to legacy device](#)

Issuing Entity:

GS1

UDI-DI from another entity

UDI-DI from another entity (secondary) applicable:

No

Selected nomenclature codes

Code L010101 MONOBLOCK SURGICAL SCALPELS, REUSABLE

Trade name

Trade name applicable:

No

Reference/Catalogue number:

BRB-CECP-2

Is the device directly marked?

Is the device directly marked?:

No

Quantity of device:

1

**NOTE**

See below for the devices where Master UDI-DI replaces UDI-DI, the *Details* section for a registered device and its Master UDI-DI:

Master UDI-DI details

Version 2 [Current] | [See version history](#) | Last update date: 2024-06-21

Master UDI-DI code:

188727_00

Issuing Entity:

HIBCC

Master UDI-DI from another entity

Master UDI-DI from another entity (secondary) applicable:

No

Selected nomenclature codes

Code G030299 DIGESTIVE ENDOSCOPY, HAEMOSTASIS DEVICES - OTHER

Code D01010102 GLUTARALDEHYDE, ACIDIC SOLUTION FOR THE DISINFECTION OF MEDICAL DEVICES

Trade name

Trade name applicable:

Yes

Trade name:

aaaaaaaaaa v2

Reference/Catalogue number:

0101912

Is the device directly marked?

Is the device directly marked?:

No

Quantity of device:

1

Playground

Type of UDI-PI

Expiration date:	Yes
------------------	-----

Additional product description:	Description_Generic_EN [EN], Description_FR [FR]
---------------------------------	---

URL for additional information (as electronic instructions for use):	www.yoursite.com/
--	-------------------

Status of the UDI-DI/Device

UDI-DI/Device status:	On the EU market
-----------------------	------------------

Clinical size

Clinical size applicable:	Yes
---------------------------	-----

Clinical size #1:	(Type): Acidity, (Precision): Value, (Value): 4.0, (Measure unit): Adult
-------------------	--

Labelled as single use

Labelled as single use:	No
-------------------------	----

Maximum number of reuses applicable:	No
--------------------------------------	----

Maximum number of reuses:	-
---------------------------	---

Need for sterilisation before use:	No
------------------------------------	----

Device labelled as sterile:	No
-----------------------------	----

Containing latex:	No
-------------------	----

The *UDI-DI/Device sub-status* subsection will become visible under the *UDI-DI/Device status* subsection once a final Field Safety Notice (FSN – Vigilance module) has been registered for the selected UDI-DI/EUDAMED ID referenced in the corresponding Field Safety Corrective Action (FSCA – Vigilance module).

Playground

**NOTE**

The sub-status of the device will be set to *Field safety corrective action initiated* if any of the following manufacturer actions are selected in the corresponding FSCA:

- IFU or labeling change
- Software Upgrade
- On-site modification/inspection by
- Customer information only
- Other

The sub-status of the device will be set to *Recalled* if any of the following manufacturer actions are selected in the corresponding FSCA:

- Product Removal - Partial Recall (Lot/Batch/Model)
- Product Removal - Full Recall

Status of the UDI-DI/Device

UDI-DI/Device status:

On the EU market

UDI-DI/Device sub-status:

2024-04-10

Recalled

- FSN-2024-04-000088
- **Product Removal : Full Recall**
- **Estimated end date: 2024-04-11**

2024-04-10

Field safety corrective action initiated

- FSN-2024-04-000089
- **Estimated end date: 2024-04-16**

Playground

**NOTE**

When the FSCA status transitions to *Action completed*, the system will remove the corresponding device sub-status:

Type of UDI-PI	
Expiration date:	Yes
Additional product description:	Description_Generic_EN [EN], Description_FR [FR]
URL for additional information (as electronic instructions for use):	www.yoursite.com/
Status of the UDI-DI/Device	
UDI-DI/Device status:	On the EU market
UDI-DI characteristics	
Clinical size	
Clinical size applicable:	Yes
Clinical size #1:	(Type): Acidity, (Precision): Value, (Value): 4.0, (Measure unit): Adult

If the FSCA status referencing the device transitions to *In progress*, the sub-status will be displayed again.

CMR/Endocrine disruptor

Labelled for presence of Carcinogenic, Mutagenic and toxic to Reproduction (CMR) substances of category 1A or 1B:	Yes
---	-----

CMR substances

Category of CMR:	1A
EC#:	-
CAS#:	-
Name of the substance:	Device_Substance_Endocrine [EN]

Labelled for presence of substance(s) with endocrine-disrupting properties:	Yes
---	-----

Endocrine-disrupting properties

EC#:	-
CAS#:	-
Name of the substance:	Device_Substance_Endocrine [EN]

Storage/handling conditions

Storage/handling conditions, if applicable:	Yes
Storage/handling condition #1:	(Type) Protect from heat and radioactive sources - (Description) Text EN_1 [All languages]

Critical warnings or contra-indications

Critical warnings or contra-indications, if applicable:Yes

Critical warning #1:(Type) Do not resterilize - (Description) CW Text [All languages]

Critical warning #2:(Type) Biological risks - (Description) CW Text 2 [All languages]

Reprocessed single use device:No

Intended purpose other than medical (Annex XVI):Yes

Brain electrostimulation

Information on substances

Presence of a substance which, if used separately, may be considered to be a medicinal product:-

Presence of a substance which, if used separately, may be considered to be a medicinal product derived from human blood or human plasma:Yes

INN Name:-

Name of the substanceDevice_Substance_Human_Product

LanguageEnglish

Related Device

This device is not currently linked with any other devices

• Product original manufacturer:

Product original manufacturer

Version 1 [Current] | Last update date: 2024-04-15

Is the device designed and manufactured by another legal or natural person?:Yes

Original equipment manufacturer actor:

Organisation name:

Address:

Telephone number:-

Email:

Actor ID/SRN:

• Market Information:

Market Information

Version 1 | Last update date: 2024-04-15

Update countries

Member State of the placing on the EU market of the Device:Belgium

Member States where device is or is to be made available on the market:

CountryBelgium

From2015-12-10

To-

• Container Package Information:

Manage your Device information

67

Container Package Information

Version 1 | Last update date: 2024-04-10

Create new version

- [Root] UDI-DI: device-2-1 (ICCBBA) | Status: On the EU market
 - UDI-DI: boxx-1 (HIBCC) | Quantity per package: 1 (1) | Status: Not intended for the EU market
 - UDI-DI: boxx-2 (ICCBBA) | Quantity per package: 1 (1) | Status: Not intended for the EU market
 - UDI-DI: boxx-3 (ICCBBA) | Quantity per package: 1 (1) | Status: On the EU market
 - UDI-DI: bbox-3-1 (ICCBBA) | Quantity per package: 1 (1) | Status: No longer placed on the EU market

 **NOTE**
Container Package Information section for a registered Master UDI-DI:

Container Package Information

Version 1 | Last update date: 2024-06-17

Create new version

- [Root] **Master** UDI-DI: 188727_00 (HIBCC) | Status: On the EU market
 - **Master** UDI-DI: ICC-919181 (ICCBBA) | Quantity per package: 10 (10) | Status: On the EU market

5.2.3 Update (create a new version) for a device and its UDI-DI/EUDAMED ID

VIDEO: UDI assignment and updates

Please note that this video does not contain sound.



Follow the steps in section [Manage your device UDI-DI/EUDAMED ID details \[58\]](#) to view a device and its UDI-DI/EUDAMED ID.

1. Once inside the details of the selected UDI-DI, click **Create new version** and proceed to update:

[See UDI-DI\(s\) list \(2\)](#) [Next UDI-DI >](#)

UDI-DI data

Version 1 [Current] | Last update date: 2021-06-10

Discard

Create new version

UDI-DI code:

12212121

Issuing Entity:

HIBCC

UDI-DI from another entity

UDI-DI from another entity (secondary) applicable:

No

Selected nomenclature codes

Code A01010102 HYPODERMIC NEEDLES FOR PEN

UDI-DI from another entity (secondary) applicable

Yes ☐ No ☒

UDI-DI from another entity is required unless you select the option - No

* Enter a nomenclature code (EMDN code):

B|

I

Find

B01

clature

Selected nomenclature codes

Code A01010102 HYPODERMIC NEEDLES FOR PEN

Remove nomenclature code

Trade name applicable

Yes ☒ No ☐

Trade name is required unless you select the option - No

* Trade name:

Trade_Name

* Select the language:

All languages

+ Add a trade name in another language

Playground

Manage your Device information

69

**NOTE**

The available options for the device status depend on the initial status of the device.

- If the initial UDI-DI status of the device is either *On the EU market* or *No longer placed on the EU market*, when updating the UDI-DI status of the device, you can select either the *On the EU market* or the *No longer placed on the EU market* status.
- If the initial UDI-DI status of the device is *Not intended for the EU market*, when updating the UDI-DI status of the device you can only select the *On the EU market* status.

**NOTE**

In the *UDI-DI status* field, if you select the *No longer placed on the EU market* status, the Market information will no longer be displayed and all container packages linked to this device will automatically be updated to the same status as the device.

[xClose](#)

Create new version of UDI-DI

You are about to create a new version of UDI-DI medical-device-01

i You have updated the device/system or procedure pack status to 'No longer placed on the EU market'. Since this device/system or procedure pack is linked to container package(s), the system will automatically change the status of the linked container package(s) to 'No longer placed on the EU market'.

Confirm

Cancel

Otherwise, if you select the *On the EU market* status, you must select a Member State in the drop-down list where the device is or has been first placed on the EU market and the Member State(s) where the device is or is to be made available. You must also manually update all container packages linked to this device.

* Member State where the Device is to or has been first placed on the EU market:

Austria ▼

* Member States where the device is or is to be made available on the market:

* [Select one or more countries >](#)

**TIP****Master UDI-DI update variation**

When creating a new version of a Master UDI-DI, the *Quantity of device* field is editable, whereas for the UDI-DI, it is not.

Basic UDI-DI 12345-family-015N

[Go to Device Details management](#)

Basic UDI-DI details Master UDI-DI(s) (1)

UDI-DI 12345-master-udi-013D [See UDI-DI\(s\) list \(1\)](#)

Master UDI-DI details

Product original manufacturer

Market Information

Container Package Information

Master UDI-DI details

Version 1 [Current] | Last update date: 2024-12-19

Master UDI-DI code: 12345-master-udi-013D

Discard [Create new version](#)

Quantity of device

Please indicate the maximum number of devices.

* Quantity of device:

10

- To finish the action you have two options:
 - Save** the updated details without submitting the new version.
 - Submit new version**, if you wish to finalise the update.

* Information on substances

Presence of a substance which, if used separately, may be considered to be a medicinal product: Yes

INN:

abc-358

[Add a substance](#)

Presence of a substance which, if used separately, may be considered to be a medicinal product derived from human blood or human plasma: No

Save [Submit new version](#) Cancel

Once you have submitted the new version, click **Confirm** in the pop-up window to finalise the update:

[Close](#)

Create new version of UDI-DI

You are about to create a new version of UDI-DI 12345-master-udi-013D

[Confirm](#) [Cancel](#)

5.2.4 Update Product original manufacturer

The *Product original manufacturer* information can be updated independently of other data in a device UDI-DI record.



NOTE

Product original manufacturer information can be updated if it was initially provided with details of an Organisation that is not a registered Actor with an Actor ID/SRN.

It **cannot** be updated if it was initially marked as *Not applicable*, or if it was specified with an Actor ID/SRN.

Follow the steps in section [Manage your device UDI-DI/EUDAMED ID details \[58\]](#) to view a UDI-DI/EUDAMED ID.

- Once inside the details of the selected UDI-DI, click **Product original manufacturer** from the list on the left (or scroll down to *Product original manufacturer*):

Basic UDI-DI data | UDI-DI(s) (2)

UDI-DI existing-PD-1 See UDI-DI(s) list (2) Next UDI-DI >

UDI-DI data

Version 1 [Current] | Last update date: -

Discard | Create new version

UDI-DI code: existing-PD-1 [Link to legacy device](#)

Issuing Entity: ICCBBA

UDI-DI from another entity

UDI-DI from another entity (secondary) applicable: No

- Click **Update** to access the *Product original manufacturer* page:

Product original manufacturer Update

Version 4 [Current] | [See version history](#) | Last update date: 2023-09-12

Is the device designed and manufactured by another legal or natural person?: Yes

Original equipment manufacturer organisation:

Organisation name: PDasOrg (3)

Address: AAA, 30, AAA, Afghanistan

Telephone number: -

Email: aaa@aaa.af

- You can **either** update the details on *Product original manufacturer*.

Natural or Legal Person update

☐ I know the Actor ID/SRN

[Change manufacturer](#)

* Name (Manufacturer Name):

PDasOrg (3)

Street information, if applicable

Yes ☒ No ☐ Street information is required unless you select the option - No

* Street: AAA Street number: 30

Address line 2:

PO box:

* City name: AAA * Postal code: AAA

* Country: Afghanistan

Telephone:

Or

- You can update the *Product original manufacturer* to an actor that is already registered in EUDAMED.
Check the box *I know the Actor ID/SRN*, enter the Actor ID/SRN or name of the *Product original manufacturer* of the device and click on **Check registry**:

Natural or Legal Person update


☒ I know the Actor ID/SRN

* Enter Actor ID/SRN or name:

Check registry

Submit **Cancel**

In the pop-up window, select the *Product original manufacturer* from the list:

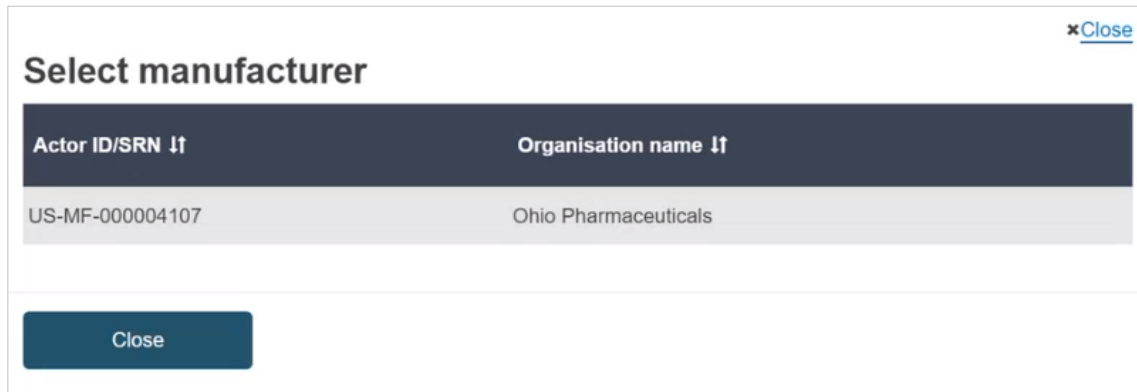

Select manufacturer ✕Close

Actor ID/SRN ↕	Organisation name ↕
US-MF-000004107	Ohio Pharmaceuticals

Close

- Click **Submit** at the bottom of the screen to finalise the update.
You will be able to see the new version created for the *Product original manufacturer* information.

**NOTE**


Once you update the *Product original manufacturer* to an actor that is already registered in EUDAMED, you will not be able to perform any further update to the Product original manufacturer via the UDI/Devices module.

5.2.5 Update Market Information

The Market Information can be updated independently of other data in a device UDI-DI record.

Follow the steps in section [Manage your device UDI-DI/EUDAMED ID details \[58\]](#) to view a UDI-DI/EUDAMED ID.

- Once inside the details of the selected UDI-DI, click **Market Information** from the list on the left (or scroll down to *Market Information*):

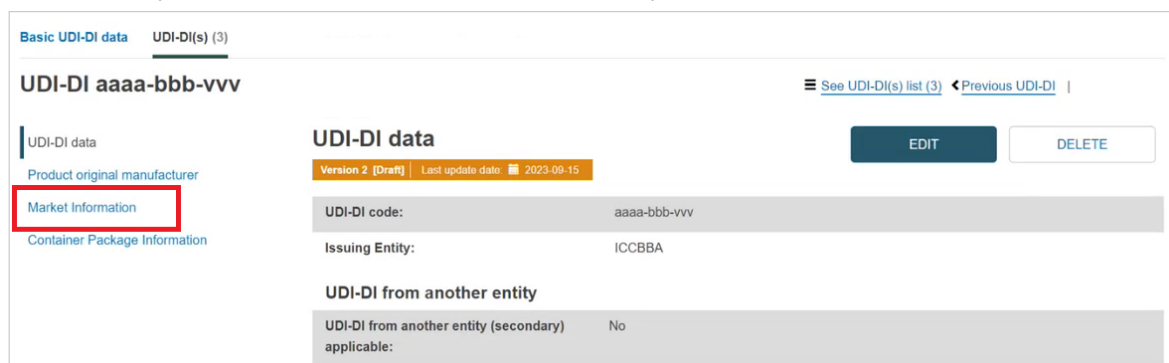

Basic UDI-DI data | UDI-DI(s) (3)

UDI-DI aaaa-bbb-vvv See UDI-DI(s) list (3) | Previous UDI-DI

UDI-DI data

Product original manufacturer

Market Information

Container Package Information

UDI-DI data Version 2 (Draft) | Last update date: 2023-09-15 EDIT DELETE

UDI-DI code: aaaa-bbb-vvv

Issuing Entity: ICCBBA

UDI-DI from another entity

UDI-DI from another entity (secondary) applicable: No

- Click **Update countries**:

Market Information Update countries

Version 1 | Last update date: 2025-07-01

Member State of the placing on the EU market of the Device:	France		
Member States where device is or is to be made available on the market:	Country	From	To
	Belgium	-	-
	France	-	-

3. Update the relevant fields under *Market Information*:

Market information update

Belgium	From		To		
		YYYY-MM-DD		YYYY-MM-DD	
Finland	From		To		
		YYYY-MM-DD		YYYY-MM-DD	
Greece	From		To		
		YYYY-MM-DD		YYYY-MM-DD	
Latvia	From		To		
		YYYY-MM-DD		YYYY-MM-DD	

* [Select one or more countries](#) >

Submit Cancel

4. Click **Submit** to finalise the update. You will be able to see the updated version of Market Information:

Market Information Update countries

Version 2 | [See version history](#) | Last update date: 2021-06-10

Member State of the placing on the EU market of the Device:	Belgium		
Member States where device is or is to be made available on the market:	Country	From	To
	Belgium	-	-
	Finland	-	-
	Greece	-	2021-06-09
	Italy	-	-
	Latvia	-	-

5.2.6 Update Container Packages

The Container Packages information can be updated independently of other data in a device UDI-DI record.

Follow the steps in section [Manage your device UDI-DI/EUDAMED ID details \[58\]](#) to view a UDI-DI/EUDAMED ID.

- Once inside the details of the selected UDI-DI, click on *Container Package information* from the list on the left (or scroll down to the relevant section):

Basic UDI-DI data UDI-DI(s) (2)

UDI-DI existing-PD-1 [See UDI-DI\(s\) list \(2\)](#) | [Next UDI-DI](#)

UDI-DI data

[Product original manufacturer](#)

[Market Information](#)

Container Package Information

UDI-DI data

Version 1 [Current] | Last update date: -

UDI-DI code: existing-PD-1 [Link to legacy device](#)

Issuing Entity: ICCBBA

UDI-DI from another entity

UDI-DI from another entity (secondary) applicable: No

[Discard](#) [Create new version](#)

2. Click **Create new version** in the *Container Package* section and proceed to update:

Container Package Information [Create new version](#)

Version 3 | [See version history](#) | Last update date: 2023-09-15

☐ [Root] UDI-DI: u-122323CiibPAY (HIBCC) | Status: On the EU market

Container package update

Container package(s)

[+ Add container package](#)

☒ [Root] UDI-DI: u-122323CiibPAY (HIBCC) | Status: On the EU market

[Submit](#) [Cancel](#)

Playground

[✕Close](#)

Add container package

 Container package UDI-DI for **UDI-DI product-original-manufacturer**

* Issuing Entity:	* Package UDI-DI code:	* Quantity per package:	Total number of devices
-		1	1

* Package status

☐ No longer placed on the EU market

☐ Not intended for EU market

☒ On the EU market

Save

Cancel

Container package update

Container package(s)

 [Add container package](#)

 [Update container package status](#)

- ☐ [Root] UDI-DI: u-123123MI9N (HIBCC) | Status: On the EU market

- ☒ UDI-DI: Cp-1-1-1 (ICCBBA) | Quantity per package: 10 (10) | Status: On the EU market

☐ UDI-DI: CP-1-1-2 (ICCBBA) | Quantity per package: 5 (50) | Status: On the EU market

Submit

Cancel

[✕Close](#)

Update container package status

 Container package UDI-DI **Cp-1-1-1**

Container package market status

☒ On the EU market ☐ No longer placed on the EU market ☐ Not intended for EU market

Confirm

Cancel

**NOTE**

Only if the status of the selected UDI-DI is *On the EU market*, will you be able to update the status of the container package. Otherwise, the options will be greyed out and you will not be able to update the status of the container package for the selected UDI-DI.

3. Click **Submit** to finalise the container package update:

Container package update

Container package(s)

 [Add container package](#)  [Update container package status](#)

☐ [Root] UDI-DI: u-123123MI9N (HIBCC) | Status: On the EU market

☒ UDI-DI: Cp-1-1-1 (ICCBBA) | Quantity per package: 10 (10) | Status: No longer placed on the EU market

☐ UDI-DI: CP-1-1-2 (ICCBBA) | Quantity per package: 5 (50) | Status: No longer placed on the EU market

Submit

Cancel

Playground

**TIP****Master UDI-DI update variation**

When creating a new version of a Master UDI-DI container package, the *Maximum quantity per package* field is editable, whereas for the UDI-DI container package, it is not:

Container package update

Container package(s)

[+ Add container package](#)

- [Root] Master UDI-DI: 12345-master-udi-013D (GS1) | Status: On the EU market
 - o Master UDI-DI: 12345-pack-mudi-01DG (GS1) | Maximum quantity per package: 10 (100) | Status: On the EU market

Submit

Cancel

Container package update

Container package(s)

[+ Add container package](#)
[↻ Update container package](#)

- [Root] Master UDI-DI: 12345-master-udi-013D (GS1) | Status: On the EU market
 - o Master UDI-DI: 12345-pack-mudi-01DG (GS1) | Maximum quantity per package: 10 (100) | Status: On the EU market

Submit

Cancel

Update container package

✕Close

Container package Master UDI-DI for **12345-pack-mudi-01DG**

* Maximum quantity per package:

Total number of devices

10

100

Container package market status

☒ On the EU market
 ☐ No longer placed on the EU market
 ☐ Not intended for the EU market

Confirm

Cancel

Container package update

Container package(s)

[+ Add container package](#)
[↻ Update container package](#)

- [Root] Master UDI-DI: 12345-master-udi-013D (GS1) | Status: On the EU market
 - o Master UDI-DI: 12345-pack-mudi-01DG (GS1) | Maximum quantity per package: 5 (50) | Status: On the EU market

Submit

Cancel

5.2.7 Discard registered devices and their UDI-DIs/ EUDAMED-IDs (and their Basic UDI-DI/EUDAMED-DI)



IMPORTANT

The *discard* operation acts as a final deactivation. A device in state *discarded* is therefore not listed and cannot be viewed in the public site of EUDAMED. However, it can be viewed by the MF (owner of the discarded device), CA and NB actors.

You may wish to discard a registered device and its UDI-DI in case you discover errors that cannot be corrected.

Follow the steps in section [Manage your device UDI-DI/EUDAMED ID details \[58\]](#) to view a registered UDI-DI/EUDAMED ID.

1. Only a user with *Confirmer* profile can discard. Once inside the details page of the selected UDI-DI, click **Discard** at the top right corner:

The screenshot shows the 'UDI-DI existing-PD-1' details page. On the right side, there are two buttons: 'Discard' and 'Create new version'. The 'Discard' button is highlighted with a red rectangular box. Above the buttons, there is a link 'See UDI-DI(s) list (2)' and a 'Next UDI-DI' link. The page also displays various data fields for the UDI-DI, including 'UDI-DI code', 'Issuing Entity', and 'UDI-DI from another entity'.


2. Confirm your intention to discard the registered UDI-DI:

The screenshot shows a confirmation dialog box titled 'Discard UDI-DI'. The text inside reads: 'Details of the UDI-DI will be Discarded (lost). The operation cannot be reverted. Do you want to finalize the operation?'. At the bottom, there are two buttons: 'Yes' and 'Cancel'. A mouse cursor is pointing at the 'Yes' button.

The UDI-DI will be discarded and will no longer be visible on the public EUDAMED website.

**CAUTION**

If the UDI-DI is the only one in this Basic UDI-DI category, the *discard* action will also discard the Basic UDI-DI. The system will alert you accordingly:

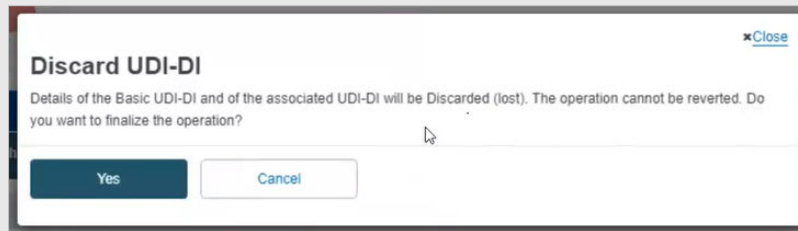

5.2.8 Link registered Regulation Device to registered Legacy Device

Follow the steps in [Manage your device UDI-DI/EUDAMED ID details \[58\]](#) and select the *Registered* option in the *State* field to manually link a registered regulation device to a registered legacy device.

1. Once inside the relevant registered regulation device click on *Link to legacy device*:

Go to Device Details management

Basic UDI-DI data UDI-DI(s) (3)

UDI-DI -device-under-regulation

See UDI-DI(s) list (3) Previous UDI-DI

UDI-DI data

Version 1 [Current] Last update date: -

Discard Create new version

UDI-DI code: -device-under-regulation **Link to legacy device**

Issuing Entity: ICCBBA

UDI-DI from another entity

UDI-DI from another entity (secondary) applicable: No

Selected nomenclature codes

Code A0101010101 HYPODERMIC SYRINGE NEEDLES, WITH SAFETY SYSTEMS

Trade name

Trade name applicable: No

Reference/Catalogue number: 12345-link-devices-SN

Is the device directly marked?

Is the device directly marked?: No

Quantity of device: 1

2. The page next contains details on the selected registered regulation device and a list with all possible compatible legacy devices to be linked to:

Playground

European Commission > EUDAMED

Home Tasks Search & view Data transfer News Help

MF (CONFIRMER) Logout

CURRENT ACTOR: Manufacturer, NL-MF-000000041, Medical Device Manufacturer [Netherlands] Notifications

Link to a legacy device

[Go back to view details page](#)

-device-under-regulation

Basic UDI-DI code:	12345-link-devices-SN
Reference/Catalogue number:	12345-link-devices-SN
Trade name:	-
UDI-DI code:	-device-under-regulation
Containing latex:	No
Labelled as single use:	Yes
Device labelled as sterile:	No
Need for sterilisation before use:	No
Reprocessed single use device:	No

List of Legacy devices

The legacy devices listed below may be compatible with your regulation device and can potentially be linked to it. Once you select the device you want to link, the system will verify that the Basic UDI-DI/UDI characteristics match between the regulation device and the legacy device before creating the link.

Select the EUDAMED ID from the list or search for a specific EUDAMED ID/UDI-DI

Search

B-device-under-directives (EUDAMED) - device-under-directives - device-under-directives	^
B-PD-orgNU (EUDAMED) - D-PD-orgNU - 1237778855	^
B-PD-orgNU (EUDAMED) - D-PD-orgNU - 1237778855	^
B-12345756984170 (EUDAMED) - 12345756984170 - 789/654**89 - Aspirin	^
B-12345756984101 (EUDAMED) - 12345756984101 - 11114/4442/ - TName - 2	^
B-NL-14V6 (EUDAMED) - D-NL-14V6 - 159*4453/4478 - TName - 2	^
B-Demo/TWTU (EUDAMED) - D-Demo/TWTU - 456/789	^
B-JKLMNOLR (EUDAMED) - D-JKLMNOLR - eee456*22	^
B-89197873912008 (EUDAMED) - 89197873912008 - Link test	^
B-my-legacy (EUDAMED) - my-legacy - aaa/bnbn	^

- You can either select the desired legacy device using the search box or you can select it from the list. Select the device and click **Select this device**:

B-12345756984170 (EUDAMED) - 12345756984170 - 789/654**89 - Aspirin

EUDAMED DI code:	B-12345756984170
Reference/Catalogue number:	789/654**89
Trade name:	Aspirin Mandarin [DE]
UDI-DI / EUDAMED ID code (issuing entity):	12345756984170 (GS1)
Containing latex:	No
Labelled as single use:	No
Device labelled as sterile:	No
Need for sterilisation before use:	No
Reprocessed single use device:	No

Select this device

B-12345756984101 (EUDAMED) - 12345756984101 - 11114/4442/ - TName - 2	^
B-NL-14V6 (EUDAMED) - D-NL-14V6 - 159*4453/4478 - TName - 2	^
B-Demo/TWTU (EUDAMED) - D-Demo/TWTU - 456/789	^
B-JKLMNOLR (EUDAMED) - D-JKLMNOLR - eee456*22	^
B-89197873912008 (EUDAMED) - 89197873912008 - Link test	^

- Click **Confirm** in the pop-up window:

Link to a legacy device [Close](#)

You are about to link UDI-DI **-device-under-regulation** to a legacy device EUDAMED ID / UDI-DI **device-under-directives**

Confirm **Cancel**

**NOTE**

If some characteristics don't match, then you will not be able to link the registered regulation device to the selected legacy device:

Link to a legacy device [Close](#)

You cannot link UDI-DI **-device-under-regulation** to EUDAMED ID / UDI-DI **12345756984170**

! The following characteristics do not match

- Active device
- Presence of a substance which, if used separately, may be considered to be a medicinal product derived from human blood or human plasma
- Device intended to administer and/or remove medicinal product
- Presence of animal tissues or cells, or their derivatives
- Labelled as single use

Cancel

5. The system will redirect you back to the regulation device's page:

European Commission > EUDAMED

Home Tasks Search & view Data transfer News Help MF (CONFIRMER) Logout

CURRENT ACTOR: Manufacturer, NL-MF-000000041, Medical Device Manufacturer [Netherlands] [Notifications](#)

✓ You have successfully created a link to the related legacy device

Basic UDI-DI 12345-link-devices-SN

[Go to Device Details management](#)

Basic UDI-DI data **UDI-DI(s) (3)**

UDI-DI -device-under-regulation [See UDI-DI\(s\) list \(3\)](#) [Previous UDI-DI](#)

UDI-DI data

Product original manufacturer

Market Information

Container Package Information

UDI-DI data

Version 1 [Current] Last update date: -

UDI-DI code: -device-under-regulation

Issuing Entity: ICCBBA

UDI-DI from another entity

UDI-DI from another entity (secondary) applicable: No

Discard **Create new version**

6. You can view details on the linked legacy device by selecting the link to the legacy device under the *Related Device* section:

Product original manufacturer
Market Information
Container Package Information

medicinal product derived from human blood or human plasma:

Related Device

Related Legacy Device: [device-under-directives](#) (link to the Legacy Device)

Devices linked on: 2023-09-12

[Remove the link to this device](#)

Product original manufacturer

Is the device designed and manufactured by another legal or natural person?: No

Market Information

Version 1 | Last update date: 2023-09-12 [Update countries](#)

Member State of the placing on the EU market of the Device: Austria

Member States where device is or is to be made available on the market:	Country	From	To
	Austria	-	-

Container Package Information

No container packages added [Add a container package UDI-DI for this UDI-DI](#)

- The legacy device's page will appear. You can view the linked regulation device under the *Related Device* section:

Product original manufacturer
Market Information

Presence of a substance which, if used separately, may be considered to be a medicinal product: -

Presence of a substance which, if used separately, may be considered to be a medicinal product derived from human blood or human plasma: -

Related Device

Related Regulation Device: [-device-under-regulation](#) (link to the Regulation Device)

Devices linked on: 2023-09-12

Product original manufacturer

Is the device designed and manufactured by another legal or natural person?: No

Market Information

Version 1 | Last update date: 2023-09-12 [Update countries](#)

Member State of the placing on the EU market of the Device: Austria

Member States where device is or is to be made available on the market:	Country	From	To
	Austria	-	-



NOTE

See the [Legacy Devices - user guide](#) for further details on Legacy Devices.

5.2.9 Delete link between Regulation Device and Legacy Device

Follow the steps in [Manage your device UDI-DI/EUDAMED ID details \[58\]](#) and select the *Registered* option in the *State* field.

- Once inside the relevant registered regulation device click on *Remove the link to this device* under the *Related Device* section:

UDI-DI data

Product original manufacturer

Market Information

Container Package Information

Presence of a substance which, if used separately, may be considered to be a medicinal product derived from human blood or human plasma: -

Related Device

Related Legacy Device: [device-under-directives](#) (link to the Legacy Device)

Devices linked on: 2023-09-12

 [Remove the link to this device](#)

Product original manufacturer

Is the device designed and manufactured by another legal or natural person?: No

Market Information

Version 1 | Last update date: 2023-09-12 [Update countries](#)

Member State of the placing on the EU market of the Device: Austria

Member States where device is or is to be made available on the market:	Country	From	To
Austria		-	-

Container Package Information

No container packages added [Add a container package UDI-DI for this UDI-DI](#)

2. Click **Confirm** on the pop-up window:

[Close](#)

Link to a legacy device

You are about to link UDI-DI -**device-under-regulation** to a legacy device EUDAMED ID / UDI-DI **device-under-directives**

Confirm [Cancel](#)

**NOTE**

See the [Legacy Devices - user guide](#) for further details on Legacy Devices.

5.2.10 View historical versions of a device and its UDI-DI/EUDAMED-ID and associated entities

Follow the steps in section [Manage your device UDI-DI/EUDAMED ID details \[58\]](#) to view a UDI-DI/EUDAMED ID.

1. Once inside the details page of the selected UDI-DI, click on *See version history* at the top of the table:

UDI-DI data

Version 2 [Draft]
[See version history](#)
Last update date: 2021-05-25

EDIT

DELETE

EUDAMED ID code:	D-1231231UU
Issuing Entity:	EUDAMED
Selected nomenclature codes Code A01010102 HYPODERMIC NEEDLES FOR PEN	
Trade name	
Trade name applicable:	No
Reference/Catalogue number:	44545
URL for additional information (as electronic instructions for use):	-
Device status:	On the EU market

2. In the list of versions displayed, click on the version you wish to access:

EUDAMED DI B-1231231UU

[Go back to the current version](#)

Version history of EUDAMED ID D-1231231UU

[See all version history \(1\)](#)

Version 1 - Last update date: 2021-05-25

EUDAMED ID code:	D-1231231UU
Issuing Entity:	EUDAMED
Selected nomenclature codes Code A01010102 HYPODERMIC NEEDLES FOR PEN	
Trade name	
Trade name applicable:	No
Reference/Catalogue number:	44545
URL for additional information (as electronic instructions for use):	-
Device status:	On the EU market
Clinical size	
Clinical size applicable:	No

3. You can return to the version history list, by clicking on *See all version history* at the top right corner.

6 Manage your own System or Procedure Pack (SPP) information

6.1 Manage your SPP Basic UDI-DI details

- On the EUDAMED dashboard, click on *Manage your Basic UDI-DIs* to see a list of all your Basic UDI-DIs:

Tasks

By module, consult, verify and/or manage your own and related data (managed by your actor), depending on your profile.

System or Procedure Pack

[Register a new System Procedure Pack](#)

[Manage your Basic UDI-DIs](#)

[Manage your UDI-DIs](#)



NOTE

By default, the system displays the System or Procedure Packs in state *draft*. To see other states, use the filters.

Basic UDI-DI management for SPP

[Go to device management](#) [Register new System or Procedure Pack](#)

Filter ▼

Active filters:

State: [Registered](#) System or Procedure Pack: [All](#) [Clear all filters](#)

Showing 1 to 3 of 3 entries Show 20 entries per page

Basic UDI-DI code IT	UDI-DI(s) IT	Device model IT	Device Name IT	Risk class IT	Type IT	Date IT	State	Actions
44444SP_Shr_1VM	1	-	SPP_Shr_1	Class I	PP	2021-06-29	Registered	...
9970314941ShnyaHL16E	1	-	System test1	Class I	S	2021-05-14	Registered	...
9970314941ShnyaHL	1	-	Test ONE	Class I	PP	2021-05-14	Registered	...

- Click on the three dots of the selected entry and then click on *View data* from the menu:

Showing 1 to 3 of 3 entries

Show entries per page

Basic UDI-DI code	UDI-DI(s)	Device model	Device Name	Risk class	Type	Date	State	Actions
44444SSP_Shr_1VM	1	-	SPP_Shr_1	Class I	PP	2021-06-29	Registered	...
9970314941ShriyaHL16E	1	-	System test1	Class I	S	2021-05-		View Data
9970314941ShriyaHL	1	-	Test ONE	Class I	PP	2021-05-		View all UDI-DIs for this Basic UDI-DI Add a UDI-DI for a Basic UDI-DI

3. A *Details* summary of your System or Procedure Pack is displayed:

Basic UDI-DI 44444SSP_Shr_1VM

[Go to UDI-DI/EUDAMED DI management](#)

Basic UDI-DI data UDI-DI(s) (1)

Basic UDI-DI data

Basic UDI-DI data Create new version

Version 1 [Current] | Last update date: 2021-05-17

Applicable regulation:	MDR (REGULATION (EU) 2017/745 on medical devices)	
Basic UDI-DI code:	44444SSP_Shr_1VM	
Issuing Entity:	GS1	
Risk class:	Class I	
Indication of medical purpose:	Indication of medical purpose	Language
	SPPP test 1	Croatian
Name:	SPP_Shr_1	

6.1.1 Delete a SPP draft Basic UDI-DI

Follow the steps in section [Manage your SPP Basic UDI-DI details \[88\]](#) to view a Draft Basic UDI-DI:

Basic UDI-DI management for SPP

[Go to device management](#) Register new System or Procedure Pack

Filter

Active filters: State: Draft System or Procedure Pack: All [Clear all filters](#)

Showing 1 to 4 of 4 entries

Show entries per page

Basic UDI-DI code	UDI-DI(s)	Device model	Device Name	Risk class	Type	Date	State	Actions
12344676768687687JC	0	-	name	Class I	S	2021-06-22	1st Draft	...
12344767686867QH	0	-	system pack name	Class IIa	S	2021-06-		View Data
123454323234324XU	0	rferfrefre	vddgv	Class I	PP	2021-06-		Edit Data
1212112121212DL	0	-		-	PP	2021-06-		View all UDI-DIs for this Basic UDI-DI

- Once inside the draft, click **Delete**:

Basic UDI-DI 12344676768687687JC

[Go to UDI-DI/EUDAMED DI management](#)

Basic UDI-DI data UDI-DI(s) (0)

Basic UDI-DI data Edit Delete

Applicable regulation:	MDR (REGULATION (EU) 2017/745 on medical devices)	
Basic UDI-DI code:	12344676768687687JC	
Issuing Entity:	GS1	
Risk class:	Class I	
Indication of medical purpose:	Indication of medical purpose	Language
	indication	English
Name:	name	

- Confirm the deletion in the pop-up window:

Delete Basic UDI-DI ✕Close

Delete Basic UDI-DI and all its related elements? Basic UDI-DI has no associated UDI-DIs.
Continue operation?

Yes Cancel

6.1.2 Update SPP Basic UDI-DI

Follow the steps in section [Manage your SPP Basic UDI-DI details \[88\]](#) to view a Basic UDI-DI:

Basic UDI-DI management for SPP

[Go to device management](#) Register new System or Procedure Pack

Filter ▼

Active filters:
State: Registered System or Procedure Pack: All [Clear all filters](#)

Showing 1 to 3 of 3 entries Show 20 entries per page

Basic UDI-DI code	UDI-DI(s)	Device model	Device Name	Risk class	Type	Date	State	Actions
4444SPP_Shr_1VM	1	-	SPP_Shr_1	Class I	PP	2021-05-17	Registered	...
9970314941ShriyaHL16E	1	-	System test1	Class I	S	2021-05-		View Data View all UDI-DIs for this Basic UDI-DI Add a UDI-DI for a Basic UDI-DI
9970314941ShriyaHL	1	-	Test ONE	Class I	PP	2021-05-		

- Once inside the *Details* page of the relevant Basic UDI-DI, click **Create new version**:

Basic UDI-DI 44444SSP_Shr_1VM

[Go to UDI-DI/EUDAMED DI management](#)

Basic UDI-DI data UDI-DI(s) (1)

Basic UDI-DI data

Basic UDI-DI data Create new version

Version 1 [Current] | Last update date: 2021-05-17

Applicable regulation:	MDR (REGULATION (EU) 2017/745 on medical devices)	
Basic UDI-DI code:	44444SSP_Shr_1VM	
Issuing Entity:	GS1	
Risk class:	Class I	
Indication of medical purpose:	Indication of medical purpose	Language
	SPPP test 1	Croatian
Name:	SPP_Shr_1	

2. Update the desired details.



NOTE

Only some details can be updated depending on the actor's specifics:

44444SSP_Shr_1VM [version: 2]

Create a new version of 44444SSP_Shr_1VM

Risk class: Class I

* Indication of medical purpose:

SPPP test 1

* Select the language:

Greek

+ Add another indication of medical purpose

* Device Name:

SPP_Shr_1

Save Submit new version Cancel

3. To finish the action you have two options:
- Click **Save** to save the updated details without submitting the new version.
 - Click **Submit new version** if you wish to submit it.

Alternatively, click **Cancel** to cancel the update.

Save Submit new version Cancel

4. After you have submitted the new version, you can see the update under the Basic UDI-DI details:

Basic UDI-DI 44444SSP_Shr_1VM

[Go to UDI-DI/EUDAMED DI management](#)

Basic UDI-DI data **UDI-DI(s) (1)**

Basic UDI-DI data

Basic UDI-DI data [Create new version](#)

Version 2 [Current] | [See version history](#) | Last update date: 2021-06-29

Applicable regulation:	MDR (REGULATION (EU) 2017/745 on medical devices)	
Basic UDI-DI code:	44444SSP_Shr_1VM	
Issuing Entity:	GS1	
Risk class:	Class I	
Indication of medical purpose:	Indication of medical purpose	Language
	SPPP test 1	Greek
Name:	SPP_Shr_1	

6.1.3 View SPP Basic UDI-DI historical versions

Follow the steps in section [Manage your SPP Basic UDI-DI details \[88\]](#) to view a Basic UDI-DI.

Once inside the *Details* page for the selected Basic UDI-DI, click *See version history* at the top of the table:

Basic UDI-DI 44444SSP_Shr_1VM

[Go to UDI-DI/EUDAMED DI management](#)

Basic UDI-DI data **UDI-DI(s) (1)**

Basic UDI-DI data

Basic UDI-DI data [Create new version](#)

Version 2 [Current] | [See version history](#) | Last update date: 2021-06-29

Applicable regulation:	MDR (REGULATION (EU) 2017/745 on medical devices)	
Basic UDI-DI code:	44444SSP_Shr_1VM	
Issuing Entity:	GS1	
Risk class:	Class I	
Indication of medical purpose:	Indication of medical purpose	Language
	SPPP test 1	Greek
Name:	SPP_Shr_1	

To return, click **Go back to the current version**:

Playground

Basic UDI-DI 44444SSP_Shr_1VM

[Go back to the current version](#)

Version history of Basic UDI-DI 44444SSP_Shr_1VM

[See all version history \(1\)](#)

Version 1 - Last update date: 2021-05-17

Basic UDI-DI identification

Applicable regulation: MDR (REGULATION (EU) 2017/745 on medical devices)

Basic UDI-DI code: 44444SSP_Shr_1VM

Issuing Entity: GS1

System or Procedure Pack type: Procedure Pack

Risk class: Class I

Indication of medical purpose:	Indication of medical purpose	Language
	SPPP test 1	Croatian

Name: SPP_Shr_1

6.2 Manage your SPP UDI-DI details

- On the EUDAMED dashboard, click *Manage your UDI-DIs* to see the list:

Tasks

By module, consult, verify and/or manage your own and related data (managed by your actor), depending on your profile.

System or Procedure Pack

[Register a new System Procedure Pack](#)[Manage your Basic UDI-DIs](#)[Manage your UDI-DIs](#)

- To find the relevant UDI-DI, click the **Filter** button and choose the right parameters:

UDI-DI details management for SPP

[Go to Basic UDI-DI management for SPP](#)

Filter ▼

Active filters:

State: Registered [Clear all filters](#)

Showing 1 to 3 of 3 entries Show 20 entries per page

UDI-DI code ID	Trade name ID	Reference/Catalogue number ID	Nomenclature code ID	Sterile ID	Date ID	Status	State	Actions
▼ Basic UDI-DI: 44444SSP_Shr_1VM, Device Name: SPP_Shr_1, Class I, Type PP, MDR (REGULATION (EU) 2017/745 on medical devices) Add a new UDI-DI								
44444SSP_Shr_1VM		SPPP_Shr_1			2021-05-17	On the EU market	Registered	...
▼ Basic UDI-DI: 9970314941ShriyaHL16E, Device Name: System test1, Class I, Type S, MDR (REGULATION (EU) 2017/745 on medical devices) Add a new UDI-DI								
34675806754T9	system 1	543			2021-05-14	On the EU market	Registered	...
▼ Basic UDI-DI: 9970314941ShriyaHL, Device Name: Test ONE, Class I, Type PP, MDR (REGULATION (EU) 2017/745 on medical devices) Add a new UDI-DI								
997031494145675552	trade1	34234			2021-05-14	On the EU market	Registered	...

**NOTE**

By default, the Basic UDI-DIs/EUDAMED DIs listed are the ones in *draft* state. To retrieve other states, use the filters.

- Click on the three dots of the desired entry and then click on *View data* from the menu:

Show entries per page

Status	State	Actions
+ Add a new UDI-DI		
On the EU market	Registered	...
+ Add a new UDI-DI		
On the EU market	Registered	...
+ Add a new UDI-DI		
On the EU market	Registered	...

- A summary of the details concerning your chosen SPP UDI-DI will be displayed:

Basic UDI-DI 44444SSP_Shr_1VM

[Go to device management](#)

Basic UDI-DI data UDI-DI(s) (1)

UDI-DI 44444SSP_Shr_1VM [See UDI-DI\(s\) list \(1\)](#)

UDI-DI data

Container Package Information

UDI-DI data

Version 1 [Current] | Last update date: 2021-05-17

UDI-DI code: 44444SSP_Shr_1VM

Issuing Entity: HIBCC

UDI-DI from another entity

UDI-DI from another entity (secondary) applicable: No

Selected nomenclature codes

Code A010204 NEEDLES AND KITS - AMNIOCENTESIS

Trade name

Trade name applicable: No

Reference/Catalogue number: SPPP_Shr_1

Type of UDI-PI

Manufacturing date: Yes

Additional product description: test [BG]

URL for additional information (as electronic instructions for use): -

UDI-DI status: On the EU market

Need for sterilisation before use: No

Device labelled as sterile: No

[Discard](#) [Create new version](#)

6.2.1 Delete SPP draft UDI-DI

Follow the steps in section [Manage your SPP UDI-DI details \[93\]](#) to view a draft UDI-DI.

1. Once inside the draft, click **Delete**:

Basic UDI-DI data UDI-DI(s) (1)

UDI-DI 34675806754T9 See UDI-DI(s) list (1)

UDI-DI data Version 2 [Draft] | See version history | Last update date: 2021-07-02 EDIT DELETE

Container Package Information

UDI-DI data

UDI-DI code: 34675806754T9

Issuing Entity: HIBCC

UDI-DI from another entity

UDI-DI from another entity (secondary) applicable: No

Selected nomenclature codes

Code: A010102 BUTTERFLY NEEDLES

Trade name

Trade name applicable: Yes

Trade name: system 1All languages

Reference/Catalogue number: 543

Type of UDI-PI

Serial number: Yes

Manufacturing date: Yes

Additional product description: test 1 for SPPP System [BG]

URL for additional information (as electronic instructions for use): -

UDI-DI status: On the EU market

2. Confirm the deletion in the pop-up window:

Delete UDI-DI ✕Close

Delete the Draft version of UDI-DI?

Yes Cancel

6.2.2 Update SPP UDI-DI

Follow the steps in [Manage your SPP UDI-DI details \[93\]](#) to view a UDI-DI:

Playground

Basic UDI-DI management for SPP

[Go to device management](#) [Register new System or Procedure Pack](#)

Filter ▼

Active filters: State: Registered System or Procedure Pack: All [Clear all filters](#)

Showing 1 to 3 of 3 entries Show 20 entries per page

Basic UDI-DI code	UDI-DI(s)	Device model	Device Name	Risk class	Type	Date	State	Actions
44444SSP_Shr_1VM	1	-	SPP_Shr_1	Class I	PP	2021-05-17	Registered	...
9970314941ShriyaHL16E	1	-	System test1	Class I	S	2021-05-		View Data
9970314941ShriyaHL	1	-	Test ONE	Class I	PP	2021-05-		View all UDI-DIs for this Basic UDI-DI Add a UDI-DI for a Basic UDI-DI

- Once inside the details of the chosen UDI-DI, click **Create new version** at the top right corner:

Basic UDI-DI 44444SSP_Shr_1VM

[Go to UDI-DI/EUDAMED DI management](#)

Basic UDI-DI data UDI-DI(s) (1)

Basic UDI-DI data

Version 1 [Current] | Last update date: 2021-05-17

[Create new version](#)

Applicable regulation:	MDR (REGULATION (EU) 2017/745 on medical devices)	
Basic UDI-DI code:	44444SSP_Shr_1VM	
Issuing Entity:	GS1	
Risk class:	Class I	
Indication of medical purpose:	Indication of medical purpose	Language
	SPPP test 1	Croatian
Name:	SPP_Shr_1	

- Update the necessary details.

**NOTE**

Only some details can be updated depending on the actor's specifics:

Create a new version of UDI-DI 4444SSP_Shr_1VM [version: 2]

UDI-DI: 4444SSP_Shr_1VM

UDI-DI from another entity (secondary) applicable
 Yes ☒ No UDI-DI from another entity is required unless you select the option - No

* Enter a nomenclature code (EMDN code):
 Find

[Advanced search of device nomenclature](#)

Selected nomenclature codes
 Code A010204 NEEDLES AND KITS - AMNIOCENTESIS Remove nomenclature code

Trade name applicable
 Yes ☒ No Trade name is required unless you select the option - No

Reference/catalogue number: SPPP_Shr_1

Type of UDI-PI
 * Manufacturing date: Yes

* Additional product description:

* Select the language:
 Bulgarian × ▼

+ [Add additional product description in another language](#)

3. To finish the action you have two options:
- Click **Save** to save the updated details without submitting the new version.
 - Click **Submit new version**, if you wish to submit it.

Otherwise click **Cancel** to cancel the update.

Save Submit new version Cancel

6.2.3 Update SPP Container Packages

The Container Packages information can be updated independently of other data in a System Procedure Pack (SPP) UDI-DI.

Follow the steps in section [Manage your SPP UDI-DI details \[93\]](#) to view a specific UDI-DI:

Basic UDI-DI 44444SSP_Shr_1VM

[Go to device management](#)

Basic UDI-DI data UDI-DI(s) (1)

UDI-DI 44444SSP_Shr_1VM [See UDI-DI\(s\) list \(1\)](#)

UDI-DI data

Container Package Information

UDI-DI data [Discard](#) [View latest draft version](#)

Version 1 [Current] | Last update date: 2021-05-17

UDI-DI code: 44444SSP_Shr_1VM

Issuing Entity: HIBCC

UDI-DI from another entity

UDI-DI from another entity (secondary) applicable: No

Selected nomenclature codes

Code A010204 NEEDLES AND KITS - AMNIOCENTESIS

1. Click *Container Package information* from the list on the left (or scroll down to the relevant section):

Basic UDI-DI data UDI-DI(s) (1)

UDI-DI 44444SSP_Shr_1VM

UDI-DI data

Container Package Information

2. Click **Create new version** in the *Container Package* section:

Container Package Information [Create new version](#)

Version 3 | [See version history](#) | Last update date: 2023-09-15

☐ [Root] UDI-DI: u-122323CiibPAY (HIBCC) | Status: On the EU market

3. Click *Add container package* to add new information about the packaging format of the SPP:

Playground

Container package update

Container package(s)

 [Add container package](#)

☒ [Root] UDI-DI: u-122323CilbPAY (HIBCC) | Status: On the EU market

4. Insert the package details in the pop-up window and click **Save**:

 [Close](#)

Add container package

 Container package UDI-DI for UDI-DI product-original-manufacturer

* Issuing Entity:	* Package UDI-DI code:	* Quantity per package:	Total number of devices
-		1	1

* Package status

☐ No longer placed on the EU market
☐ Not intended for EU market
☒ On the EU market

6.2.4 Discard SPP registered UDI-DIs

Follow the steps in section [Manage your SPP UDI-DI details \[93\]](#) to view a chosen Registered UDI-DI:

Playground

UDI-DI details management for SPP

[Go to Basic UDI-DI management for SPP](#)

Filter ▼

Active filters:
State: Registered [Clear all filters](#)

Showing 1 to 3 of 3 entries Show 20 entries per page

UDI-DI code IT	Trade name IT	Reference/Catalogue number IT	Nomenclature code IT	Sterile IT	Date IT	Status	State	Actions
Basic UDI-DI: 44444SSP_Shr_1VM, Device Name: SPP_Shr_1, Class I, Type PP, MDR (REGULATION (EU) 2017/745 on medical devices) Add a new UDI-DI								
44444SSP_Shr_1VM		SPPP_Shr_1			2021-05-17	On the EU market	Registered	...
Basic UDI-DI: 9970314941ShriyaHL16E, Device Name: System test1, Class I, Type S, MDR (REGULATION (EU) 2017/745 on medical devices) Add a new UDI-DI								
34675806754T9	system 1	543			2021-05-14	On the EU market	Registered	...
Basic UDI-DI: 9970314941ShriyaHL, Device Name: Test ONE, Class I, Type PP, MDR (REGULATION (EU) 2017/745 on medical devices) Add a new UDI-DI								
997031494145675552	trade1	34234			2021-05-14	On the EU market	Registered	...

- Once inside the *Details* page of the chosen UDI-DI, click **Discard** at the top right corner:

Basic UDI-DI 44444SSP_Shr_1VM

[Go to device management](#)

Basic UDI-DI data UDI-DI(s) (1)

UDI-DI 44444SSP_Shr_1VM [See UDI-DI\(s\) list \(1\)](#)

UDI-DI data [Container Package Information](#)

UDI-DI data [Discard](#) [Create new version](#)

Version 1 [Current] | Last update date: 2021-05-17

UDI-DI code: 44444SSP_Shr_1VM

Issuing Entity: HIBCC

UDI-DI from another entity

UDI-DI from another entity (secondary) applicable: No

Selected nomenclature codes

Code A010204 NEEDLES AND KITS - AMNIOCENTESIS

Trade name

Trade name applicable: No

Reference/Catalogue number: SPPP_Shr_1

Type of UDI-PI

Manufacturing date: Yes

Additional product description: test [BG]

URL for additional information (as electronic instructions for use): -

UDI-DI status: On the EU market

Need for sterilisation before use: No

Device labelled as sterile: No

UDI-DI data [See UDI-DI\(s\) list \(1\)](#) [Discard](#) [Create new version](#)

Version 1 [Current] | Last update date: 2021-05-17

UDI-DI code: 44444SSP_Shr_1VM

Issuing Entity: HIBCC

UDI-DI from another entity

- Confirm your intention to discard the record in the pop-up window:

Discard UDI-DI [Close](#)

Details of the Basic UDI-DI and of the associated UDI-DI will be Discarded (not). The operation cannot be reverted. Do you want to finalize the operation?

[Yes](#) [Cancel](#)

6.2.5 View SPP historical versions for UDI-DI and associated entities

Follow the steps in section [Manage your SPP UDI-DI details \[93\]](#) to view a UDI-DI for the SPP.

1. Once inside the details of the chosen UDI-DI, click *See version history* at the top of the table to view a list of all past versions:

The screenshot shows the 'Basic UDI-DI data' page for '12345-test-udi-1-HL'. At the top, it says 'Version 4 [Current]' and has a link 'See version history' which is highlighted with a mouse cursor. To the right is a 'Create new version' button. Below this is a table with the following data:

Applicable regulation:	MDR (REGULATION (EU) 2017/745 on medical devices)
Basic UDI-DI code:	12345-test-udi-1-HL
Issuing Entity:	GS1
Is it a System or Procedure Pack which is a Device in itself?:	Procedure Pack which is a device in itself

Below the table is a section titled 'Basic UDI-DI 12345-test-udi-1-HL' with a button 'Go back to the current version'. Underneath is the 'Version history of Basic UDI-DI 12345-test-udi-1-HL' section, which lists three versions:

Version 3 - Last update date: 2021-06-09	>
Version 2 - Last update date: 2021-06-09	>
Version 1 - Last update date: 2021-05-03	>

2. Click on the version you wish to access to view its detailed summary:

The screenshot shows the 'Version history of Basic UDI-DI 12345-test-udi-1-HL' page. At the top, it says 'Version 2 - Last update date: 2021-06-09'. Below this is a section titled 'Basic UDI-DI identification' with the following data:


Applicable regulation:	MDR (REGULATION (EU) 2017/745 on medical devices)
Basic UDI-DI code:	12345-test-udi-1-HL
Issuing Entity:	GS1
Is it a System or Procedure Pack which is a Device in itself?:	Procedure Pack which is a device in itself

Below this is a section titled 'Risk class:' with the value 'Class IIb'. At the bottom, it says 'Implantable: No'. In the top right corner, there are links: 'See all version history (3)', 'Previous version [v1]', and 'Next version [v3]'.


You can return to the version history list by clicking on *See all version history* at the top right corner.

7 Search & View Devices and Systems or Procedure Packs

1. On the header menu, click **Search & View**, then **UDI-DIs/Devices**:

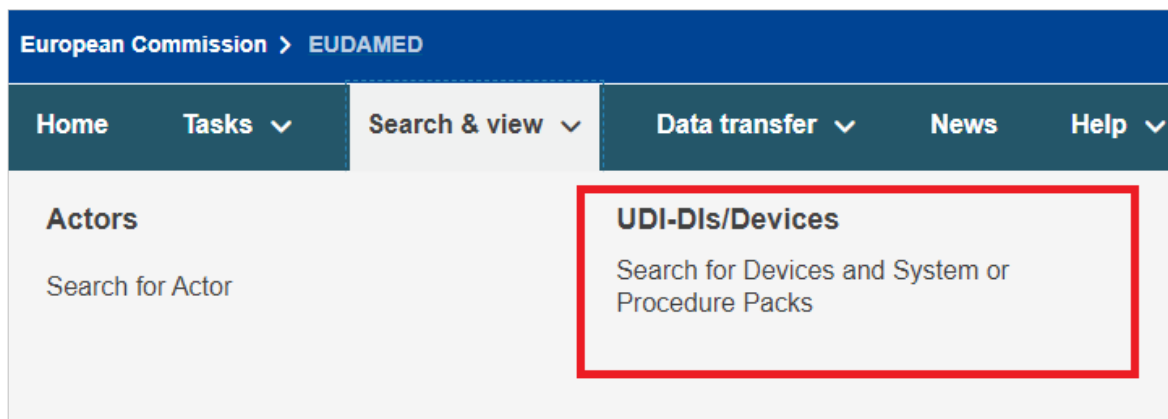

Alternatively, use the *Search & View* option available on the dashboard:

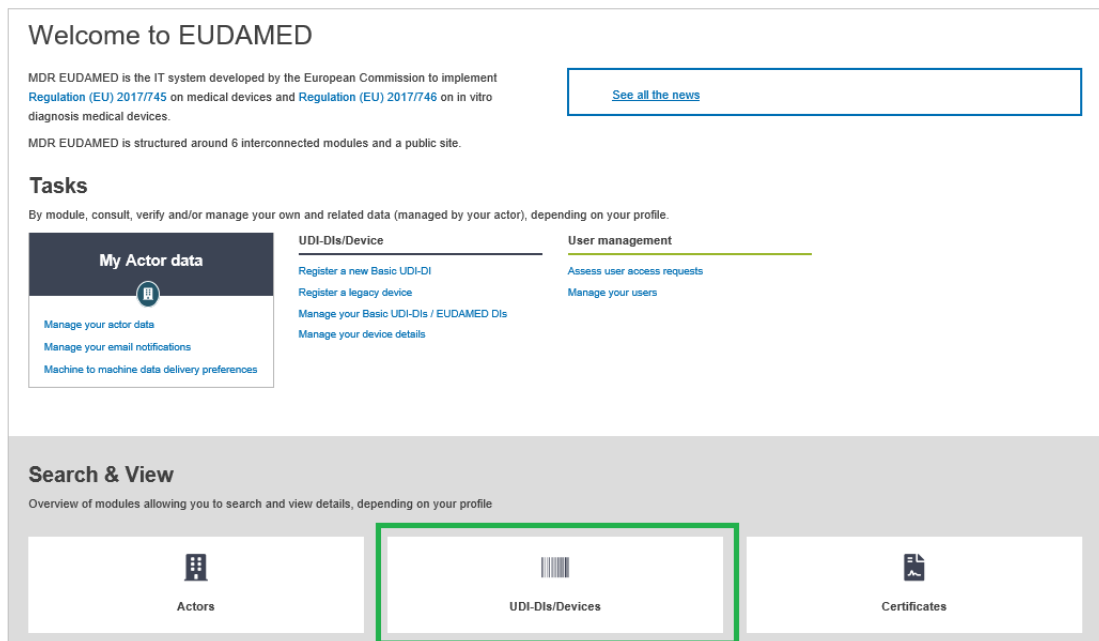

NOTE

Search and view can be accessed by all users, regardless of profile. It is possible to search and view device and SPP data from all actors in EUDAMED.

2. You can use the filters to search for *Devices*, *Systems* and/or *Procedure Packs (SPP)* registered in EUDAMED, or, in the case of Competent Authorities and Notified Bodies, those *submitted* or *discarded*:

Search Devices and System or Procedure Packs

☐ Enable search filters available for bulk XML download

(Master) UDI-DI/ EUDAMED ID:

Basic UDI-DI/ EUDAMED DI:

Status:

Sub-status:

Model:

Name:

Trade name:

Applicable regulation:

Risk class:

Nomenclature code:

Reference/Catalogue number:

Country:

Scope:

Competent Authority:

NB identification:

MF / PR Actor ID/SRN:

MF / PR Name:

AR Actor ID/SRN:

AR name:

Results option

Include historical version: ☐

3. Once you have entered your search filters, click **Search** (the record will have to match all the filters). A list of Devices (UDI-DIs/EUDAMED IDs) and/or Systems or Procedure Packs will appear if any are found (otherwise *No data available* will be displayed):

Showing 1 to 20 of 5559 entries

Show entries per page


(Master) UDI-DI code <i>1</i>	(Master) UDI-DI version	Basic UDI-DI / EUDAMED DI <i>1</i>	MF / PR Actor ID/SRN	Trade name <i>1</i>	Risk class	Date <i>1</i>	UDI-DI/Device status
188727_00	1 [Current]	777777777770UZ	NL-MF-000000041	aaaaaaaaaa	Class I	2024-06-17	On the EU market
555245841651036LM	1 [Current]	555245841651036LM	CA-MF-000006393		Class I	2024-06-14	On the EU market
4520363415562TP	1 [Current]	4520363415562TP	BE-MF-000006007		Class I	2024-06-14	On the EU market
4520363415561TM	1 [Current]	4520363415561TM	BE-MF-000006007		Class IIa	2024-06-14	On the EU market

4. Click on the UDI-DI/EUDAMED ID row of your choice to see the details:

Producer information
Producer identification Organisation name: Belgian PPA SRN: BE-PR-000000048 Address: 1 Rue H Brussels, Belgium Telephone number: - Email: contact@belgian-pp-a.be
Basic UDI-DI details Version 1 - [Current] - Last update date: 2021-03-29
Basic UDI-DI identification Applicable regulation: MDR (REGULATION (EU) 2017/745 on medical devices)
Basic UDI-DI code: ++B311X1Y2Z3PP Issuing Entity: HIBCC
System or Procedure Pack type: Procedure Pack


7.1 Search & View sub-statuses of Devices or SPPs

- On the header menu, click **Search & View**, then **UDI-DIs/Devices**:

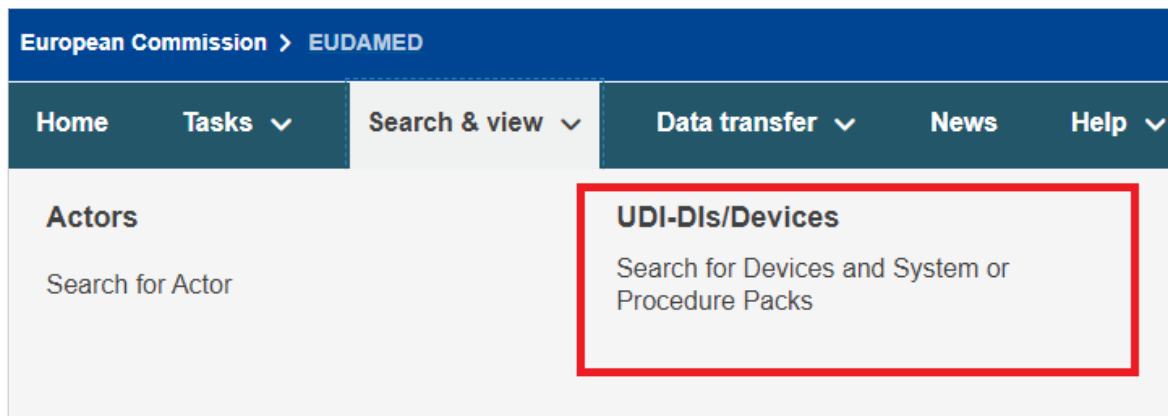

Alternatively, use the option available in the dashboard called *Search & View*:

Playground

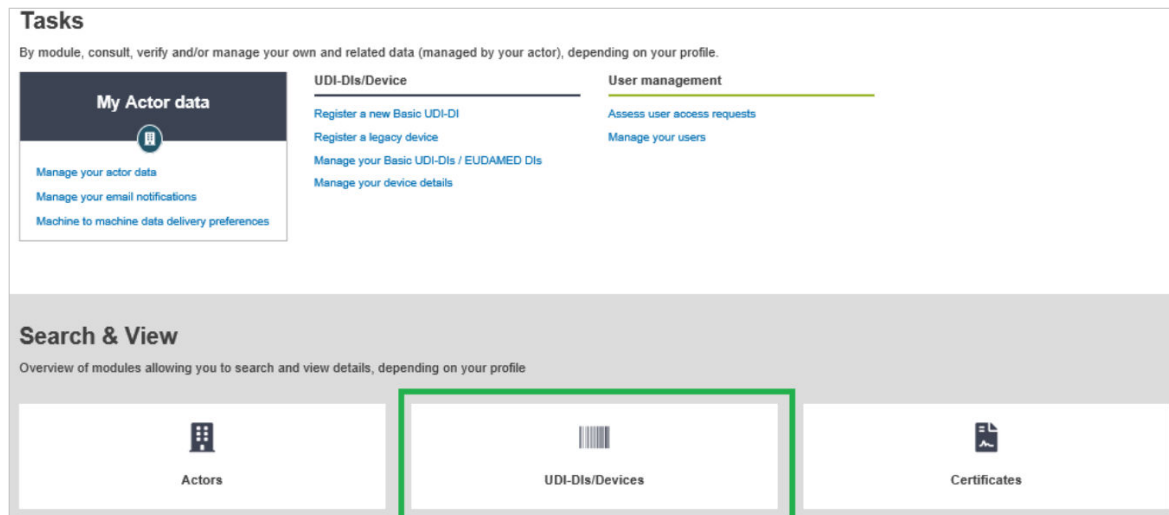

2. Select the sub-status in the dropdown list and click **Search**:

Search Devices and System or Procedure Packs

☐ Enable search filters available for bulk XML download

(Master) UDI-DI/ EUDAMED ID	Basic UDI-DI/ EUDAMED DI	Status	Sub-status
		On the EU market X v	You can select more than one value v
Model	Name	Trade name	Field Safety Corrective Action initiated
			Recalled
Applicable regulation	Risk class	Nomenclature code	
-- X v	-- X v		
Reference/Catalogue number	Country	Scope	
	-- X v	-- X v	
Competent Authority	NB identification	MF / PR Actor ID/SRN	MF / PR Name
-- X v	-- X v		
AR Actor ID/SRN	AR name		

3. A list of Devices (UDI-DIs/EUDAMED IDs) and/or Systems or Procedure Packs will appear if any are found:

Playground

Showing 1 to 20 of 39 entries

Show 20 entries per page

(Master) UDI-DI code IT	(Master) UDI-DI version	Basic UDI-DI / EUDAMED DI IT	MF / PR Actor ID/SRN	Trade name IT	Risk class	Date 1 st	UDI-DI/Device status
BRB-cd-1	1 [Current]	109784903285972P5	NL-MF-000000041		Class IIa	2024-06-11	On the EU market (Recalled)
B09DGK9T8M	1 [Current]	7486566855F8	EL-MF-000004067		Class IIb	2024-06-10	On the EU market (Field safety corrective action initiated)
gfh12867	1 [Current]	6986201dk3N	BH-MF-000006127		Class IIb	2024-05-30	On the EU market (Field safety corrective action initiated)
300524022GT	1 [Current]	300524022GT	IN-MF-000005648		Class IIb	2024-05-30	On the EU market (Recalled)
300524021GR	1 [Current]	300524021GR	IN-MF-000005648		Class IIb	2024-05-30	On the EU market (Field safety corrective action initiated)
gudi9978	1 [Current]	6986214dk4C	BH-MF-000006127		Class D	2024-05-30	On the EU market (Field safety corrective action initiated)
280524021LS	1 [Current]	280524021LS	IN-MF-000005648		Class III	2024-05-28	On the EU market (Field safety corrective action initiated)
270524015LC	1 [Current]	270524015LC	IN-MF-000005648		Class IIa	2024-05-27	On the EU market (Recalled)
270524011L4	1 [Current]	270524011L4	IN-MF-000005648		Class IIb	2024-05-27	On the EU market (Recalled)
00000069862120	1 [Current]	6986215d01KY	BH-MF-000006127		Class C	2024-05-23	On the EU market (Recalled, Field safety corrective action initiated)
00000069862113	1 [Current]	6986213d01KJ	BH-MF-000006127		Class IIb	2024-05-23	On the EU market (Field safety corrective action initiated, Recalled)
00000069862182	1 [Current]	698621d013C	BH-MF-000006127		Class IIb	2024-05-23	On the EU market (Recalled)
00000069862137	1 [Current]	698621d003A	BH-MF-000006127		Class IIb	2024-05-23	On the EU market (Field safety corrective action initiated, Recalled)
2160524011YD	1 [Current]	2160524011YD	IN-MF-000005648		Class III	2024-05-21	On the EU market (Recalled)

- Click on the UDI-DI/EUDAMED ID row of your choice to see the details. Scroll down to the *Status of the UDI-DI/Device* subsection.

Read the [View details of a registered UDI-DI/EUDAMED ID \[61\]](#) section for more details on the sub-status of a device.

7.2 Search & View historical versions of Devices or SPPs

Follow the steps in [Search & View Devices, Systems and/or Procedure Packs \[102\]](#) to search and view a Device or System or Procedure Pack.

- Inside the search page, select the filters for your search, activate the option to include historical versions (toggle just above the **Search** button) and click **Search**:

Playground

Search Devices and System or Procedure Packs

☐ Enable search filters available for bulk XML download

(Master) UDI-DI/ EUDAMED ID:

Basic UDI-DI/ EUDAMED DI:

Status: X v

Sub-status:

Model:

Name:

Trade name:

Applicable regulation: X v

Risk class: X v

Nomenclature code:

Reference/Catalogue number:

Country: X v

Scope: X v

Competent Authority: X v

NB identification: X v

MF / PR Actor ID/SRN:

MF / PR Name:

AR Actor ID/SRN:

AR name:

Results option

Include historical version: ☐

[Search](#) [Generate XML file](#) [Clear search](#)

2. The list generated will include the desired current UDI-DI as well as its versions. Click on the version you wish to view:

UDI-DI code ¹	Version Number	Basic UDI-DI code ¹	MF / PR SRN	Trade name ¹	Risk class	Date ¹	UDI-DI status
232121122132	2 [Current]	223311445578899583F	BE-PR-000000022	Trade_Name	Class I	2021-07-07	On the EU market
D-12345-bug-testFF	1 [Current]	B-12345-bug-testFF	BE-MF-000000001		Class I	2021-07-05	On the EU market
IFA0705	2 [Current]	202107052FS	BE-MF-000000001		Class III	2021-07-05	On the EU market
0705HIBCC	2 [Current]	202107051FQ	BE-MF-000000001		Class IIb	2021-07-05	On the EU market
0705HIBCC	1 [History]	202107051FQ	BE-MF-000000001		Class IIb	2021-07-05	On the EU market
IFA0705	1 [History]	202107052FS	BE-MF-000000001		Class III	2021-07-05	On the EU market
udid-36	1 [Current]	12345test-empty-langTC	BE-MF-000000001		Class I	2021-07-05	Not intended for the EU market
test-empty-lang1	1 [Current]	12345test-empty-langTC	BE-MF-000000001	trade name1	Class I	2021-07-05	Not intended for the EU market
udid-37	1 [Current]	12345empty-MLT-1NH	BE-MF-000000001		Class I	2021-07-02	Not intended for the EU market
UDID-1	2 [Current]	12345empty-MLT-1NH	BE-MF-000000001		Class I	2021-07-02	Not intended for the EU market
UDID-1	1 [History]	12345empty-MLT-1NH	BE-MF-000000001		Class I	2021-07-02	Not intended for the EU market
12123	1 [Current]	12123qqqP9	BE-MF-000000001		Class IIb	2021-07-01	On the EU market
cdc	1 [Current]	22222e1234566543e5L5	BE-MF-000000001		Class IIb	2021-06-28	On the EU market
cdc	1 [Current]	22222e1234566543eEG	BE-MF-000000001		Class IIa	2021-06-28	On the EU market
vhvf	1 [Current]	22222e12345665435T	BE-MF-000000001		Class IIb	2021-06-28	On the EU market
1234_1234_57676	1 [Current]	1212112121212121214K	BE-MF-000000001	External Implant	Class I	2021-06-22	On the EU market
11223	1 [Current]	11223qqqP5	JP-MF-000000061		Class IIa	2021-06-21	On the EU market
eeee	4 [Current]	22223434444FY	BE-MF-000000001	Trade_Name_v4	Class I	2021-06-21	On the EU market
eeee	3 [History]	22223434444FY	BE-MF-000000001	Trade_Name_v3	Class I	2021-06-21	On the EU market
eeee	2 [History]	22223434444FY	BE-MF-000000001	Trade_Name_v2	Class I	2021-06-21	On the EU market

[← Previous](#)
[1](#)
[2](#)
[3](#)
[4](#)
[5](#)
[Next →](#)

7.3 Download Devices or SPPs data in a structured format (XML)



NOTE

You can only manually bulk-download in XML your own device or system/procedure pack data if you are a manufacturer or a system/procedure pack producer.

Follow the steps in [Search & View Devices, Systems and/or Procedure Packs \[102\]](#) to search and view a device or a system or procedure pack.

1. On the *Search* page, activate the top filter (**Only enable search filters available for bulk XML download**) and enter your search criteria.

Enter the search criteria of your choice, and click **Search**:

Search Devices and System or Procedure Packs

☒ Enable search filters available for bulk XML download

(Master) UDI-DI/ EUDAMED ID 	Basic UDI-DI/ EUDAMED DI 	Status --	Sub-status You can select more than one value
Model 	Name 	Trade name 	
Applicable regulation --	Risk class --	Nomenclature code 	
Reference/Catalogue number 	Country --	Scope --	
MF / PR Actor ID/SRN MF 00000000000000000000000000000000	MF / PR Name 	AR Actor ID/SRN 	AR name

Results option

Include historical version ☐

2. Click on **Generate XML file**:




NOTE

Only what is shown on the result list will be included in the generated file and not all the results of your search. If the search yields multiple pages of results, you will need to download an XML file for each page to capture all the data.


- Confirm your action in the pop-up window:



- The system will display a success message. Click **Go to Download Management** under the question *What do you want to do now?*:

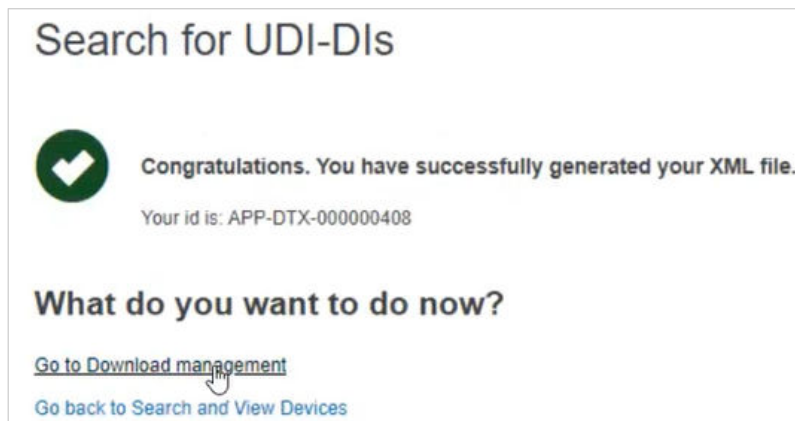

- You can download the generated XML file by clicking on it under the **Download** column:

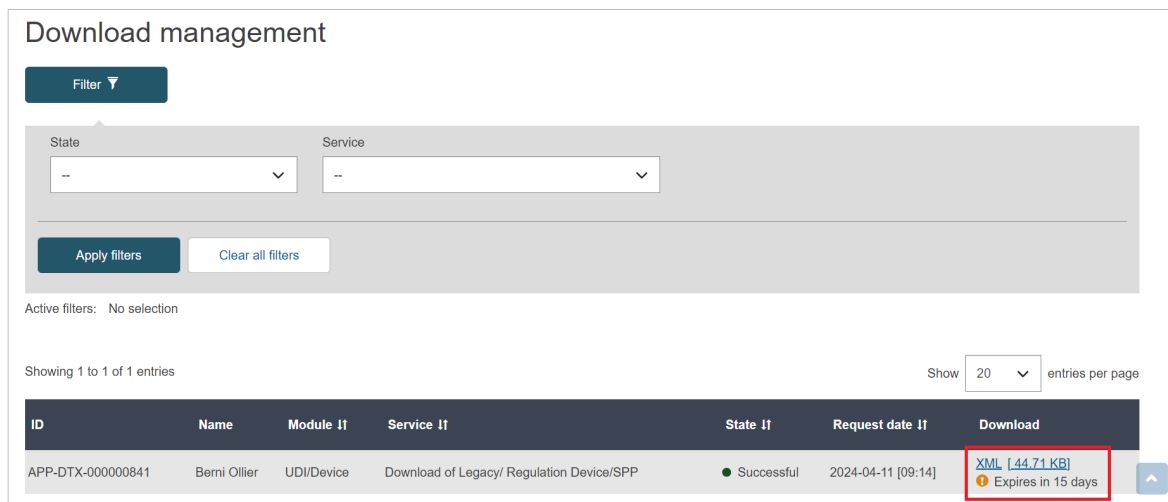

7.4 View historical versions of Basic UDI-DI/EUDAMED DI, UDI-DI/EUDAMED ID and associated entities

Follow the steps in [Search & View historical versions of Devices, System and/or Procedure Packs \[106\]](#) to view the details of a Device or System or Procedure Pack.

- Once inside the details of the chosen UDI-DI, go to the section in which you wish to view old versions (e.g. Basic UDI-DI/EUDAMED DI, UDI-DI/EUDAMED ID, Market

Information, Product original manufacturer or Container Package) and click on **See version history**:

Go back to the list

Manufacturer information

Basic UDI-DI details

UDI-DI details

Market information

Clinical Investigation(s)

Manufacturer information

Organisation name: Japanese MF A v4
Actor ID/SRN: JP-MF-000000061
Address: 1 Main Street Tokyo
Telephone number: 213 v2
Email: public-details@japanese-mf-a.com

Authorised Representative

Organisation name: Belgium AR A v6
Eudamed actor ID: BE-AR-000000021
Address: Brussels
Telephone number: -
Email: public-contact@belgium-ar-a.com

Basic UDI-DI details

Version 5 [Current] **See version history** Last update date: 2021-09-23

Basic UDI-DI identification

Applicable regulation: MDR (REGULATION (EU) 2017/745 on medical devices)

Basic UDI-DI code: 22091test23_09EC
Issuing Entity: GS1

Is it a System or Procedure Pack which is a Device in itself? No
Special device type: No

List of UDI-DIs for the Basic UDI-DI

UDI-DI details

Version 3 [Current] **See version history** Last update date: 2021-09-24

UDI-DI code: 121312_Test_AR
Issuing Entity: HIBCC

UDI-DI from another entity

UDI-DI from another entity (secondary) applicable: No

Selected nomenclature codes

Code A01010199 HYPODERMIC NEEDLES - OTHERS

Trade name

Trade name applicable: Yes

Trade name: TB_BG [BG],
TN_AR1_Croatian [HR]

Reference/Catalogue number: ref

Is the device directly marked?

Is the device directly marked?: No

Market information

Version 1 [Current] | Last update date: 2021-09-23

Member State of the placing on the EU market of the Device:	Belgium		
Member States where device is or is to be made available on the market:	Country	From	To
	Belgium	-	-
	Iceland	-	-
	Ireland	-	-
	Malta	-	-
	Netherlands	-	-

Clinical Investigation(s)

Clinical Investigation

Clinical Investigation, if applicable:	No
--	----

2. You will see, if any, a list of all old versions for the selected entity, e.g. version history of the Basic UDI-DI:

Basic UDI-DI 22091test23_09EC

[Go back to the current version](#)

Historical version for Basic UDI-DI 22091test23_09EC

Version 4 - Last update date: 2021-09-23	>
Version 3 - Last update date: 2021-09-23	>
Version 2 - Last update date: 2021-09-23	>
Version 1 - Last update date: 2021-09-23	>

3. Click on the version you wish to view to access its details:

Playground

Basic UDI-DI 22091test23_09EC

[Go back to the current version](#)

Historical version for Basic UDI-DI 22091test23_09EC

Version 3 [History] - Last update date: 2021-09-23

[See all version history \(4\)](#) [Previous version \[v2\]](#) [Next version \[v4\]](#)

Manufacturer information

Basic UDI-DI data

Clinical Investigation

List of UDI-DIs for the Basic UDI-DI

Manufacturer information

Organisation name: Japanese MF A v4
 Actor ID/SRN: JP-MF-000000061
 Address: 1 Main Street Tokyo
 Telephone number: 213 v2
 Email: public-details@japanese-mf-a.com

Authorised Representative

Organisation name: Belgium AR A v5
 Eudamed actor ID: BE-AR-000000021
 Address: Brussels
 Telephone number: -
 Email: public-contact@belgium-ar-a.com

Basic UDI-DI data

Version 3 [History] | Last update date: 2021-09-23

Basic UDI-DI identification

Applicable regulation: MDR (REGULATION (EU) 2017/745 on medical devices)

Basic UDI-DI code: 22091test23_09EC
 Issuing Entity: GS1

Is it a System or Procedure Pack which is a Device in itself? No
 Special device type: No

4. Inside a version, click on the links at the top right corner to browse through the different versions (*all versions, previous, next*):

Basic UDI-DI 22091test23_09EC

[Go back to the current version](#)

Historical version for Basic UDI-DI 22091test23_09EC

Version 3 [History] - Last update date: 2021-09-23

[See all version history \(4\)](#) [Previous version \[v2\]](#) [Next version \[v4\]](#)

Manufacturer information

Basic UDI-DI data

Clinical Investigation

List of UDI-DIs for the Basic UDI-DI

Manufacturer information

Organisation name: Japanese MF A v4
 Actor ID/SRN: JP-MF-000000061
 Address: 1 Main Street Tokyo
 Telephone number: 213 v2
 Email: public-details@japanese-mf-a.com

Authorised Representative

Organisation name: Belgium AR A v5
 Eudamed actor ID: BE-AR-000000021
 Address: Brussels
 Telephone number: -
 Email: public-contact@belgium-ar-a.com

Basic UDI-DI data

Version 3 [History] | Last update date: 2021-09-23

Basic UDI-DI identification

Applicable regulation: MDR (REGULATION (EU) 2017/745 on medical devices)

Basic UDI-DI code: 22091test23_09EC
 Issuing Entity: GS1

Is it a System or Procedure Pack which is a Device in itself? No
 Special device type: No

8 Annex – device certificate information

This Annex presents the cases in which the Certificate information needs to be provided when registering a Regulation Device and the Certificate type to be provided based on the properties of the device.

The updated versions of the tables below can also be consulted here: [Notified Bodies and Certificates module - Documentation](#)

IVDR Conformity assessments table

IVD: Device class & Certificate type		EU QMS Device or Group	EU TDA Device	EU TE Device	EU PQA Device or Group
Class D		✓ (NB)	✓ (NB, SSP, scrutiny)		
Class C	Self/near patient testing devices	✓ (NB)	✓ (NB, SSP)	✓ (SSP, scrutiny)	✓
	Companion diagnostics	✓ (NB)	✓ (NB, SSP)	✓ (SSP)	✓
	All other class C devices	✓ (SSP)		✓ (SSP)	✓
Class B	Self/near patient testing devices	✓ (NB)	✓ (NB)		
	All other class B devices	✓			
A sterile		✓			✓
29.3 par #1: MF assigns a Basic UDI-DI before it applies to a NB 29.3 par #2: NB confirms the concerned device data in registering the certificate in Eudamed. As a pre-requisite the MF provides the NB identification and certificate type information with submission of Basic UDI-DI data in Eudamed. (NB) = Same NB carries the conformity assessments.					

MDR Conformity assessments table

MDR: Applicable conformity assessments per device class (and characteristics of the device class)			EU QMS (scope is defined using devices and/or device annexes)	EU TDA (certificate scope is defined using devices)	EU TE (certificate scope is defined using devices)	EU QA (scope is defined using devices and/or device annexes)	EU PV (certificate scope is defined using devices)		
Each line represents a different path for assessing the conformity of a device.									
III	Implantable		✓ (NB)	✓ (NB, CECP, SSCP)		✓ CECP, SSCP	✓		
					✓ CECP, SSCP)			✓	
	Non implantable		✓ (NB)	✓ (NB, SSCP)					
						✓ (SSCP)	✓		✓
IIb	IIb implantable	NON sutures/staples/dental fillings/...	✓ (NB)	✓ (NB, SSCP)					
						✓ (SSCP)	✓		
		sutures/staples/dental fillings/...				✓ (SSCP)			
				✓ (SSCP)	sample/generic device group		✓ (SSCP)	✓	
	IIb non implantable	- Active devices intended to administer and/or remove a medicinal product	CECP	sample/generic device group		✓ CECP	✓		
						✓ CECP			✓
		- Non active devices - Active devices NOT intended to administer and/or remove a medicinal product	✓	sample/generic device group			✓		
						✓			✓
IIa	Implantable		✓ (SSCP)	sample/device category					
							✓ (SSCP)		✓ (SSCP)
	Non implantable		✓	sample/device category			✓		
									✓
I sterile condition/measuring function/reusable surgical instrument)			✓				✓		
III custom-made implantable (a certificate is needed only for implantable devices)									
System/Procedure pack (SPP sterilisation)			✓				✓		

29.3 par #1: MF assigns a Basic UDI-DI before it applies to a NB

29.3 par #2: NB confirms the concerned device data in registering the certificate in Eudamed. As a pre-requisite the MF provides the certificate identification information with submission of Basic UDI-DI data in Eudamed.

Devices that may require a CECP for a QMS certificate (in case there is no EU TDA certificate or EU Type examination certificate)

CECP could apply from MDR but it was agreed that CECP is never to be applied for custom-made devices

(NB) = Same NB carries the conformity assessments.

(CECP) = Should requires a CECP

SSCP is required for implantable and class III devices. If the device needs both a product and a quality certificate then the SSCP is only uploaded with the product certificate.

